


ITS.

Implants for Trauma Surgery

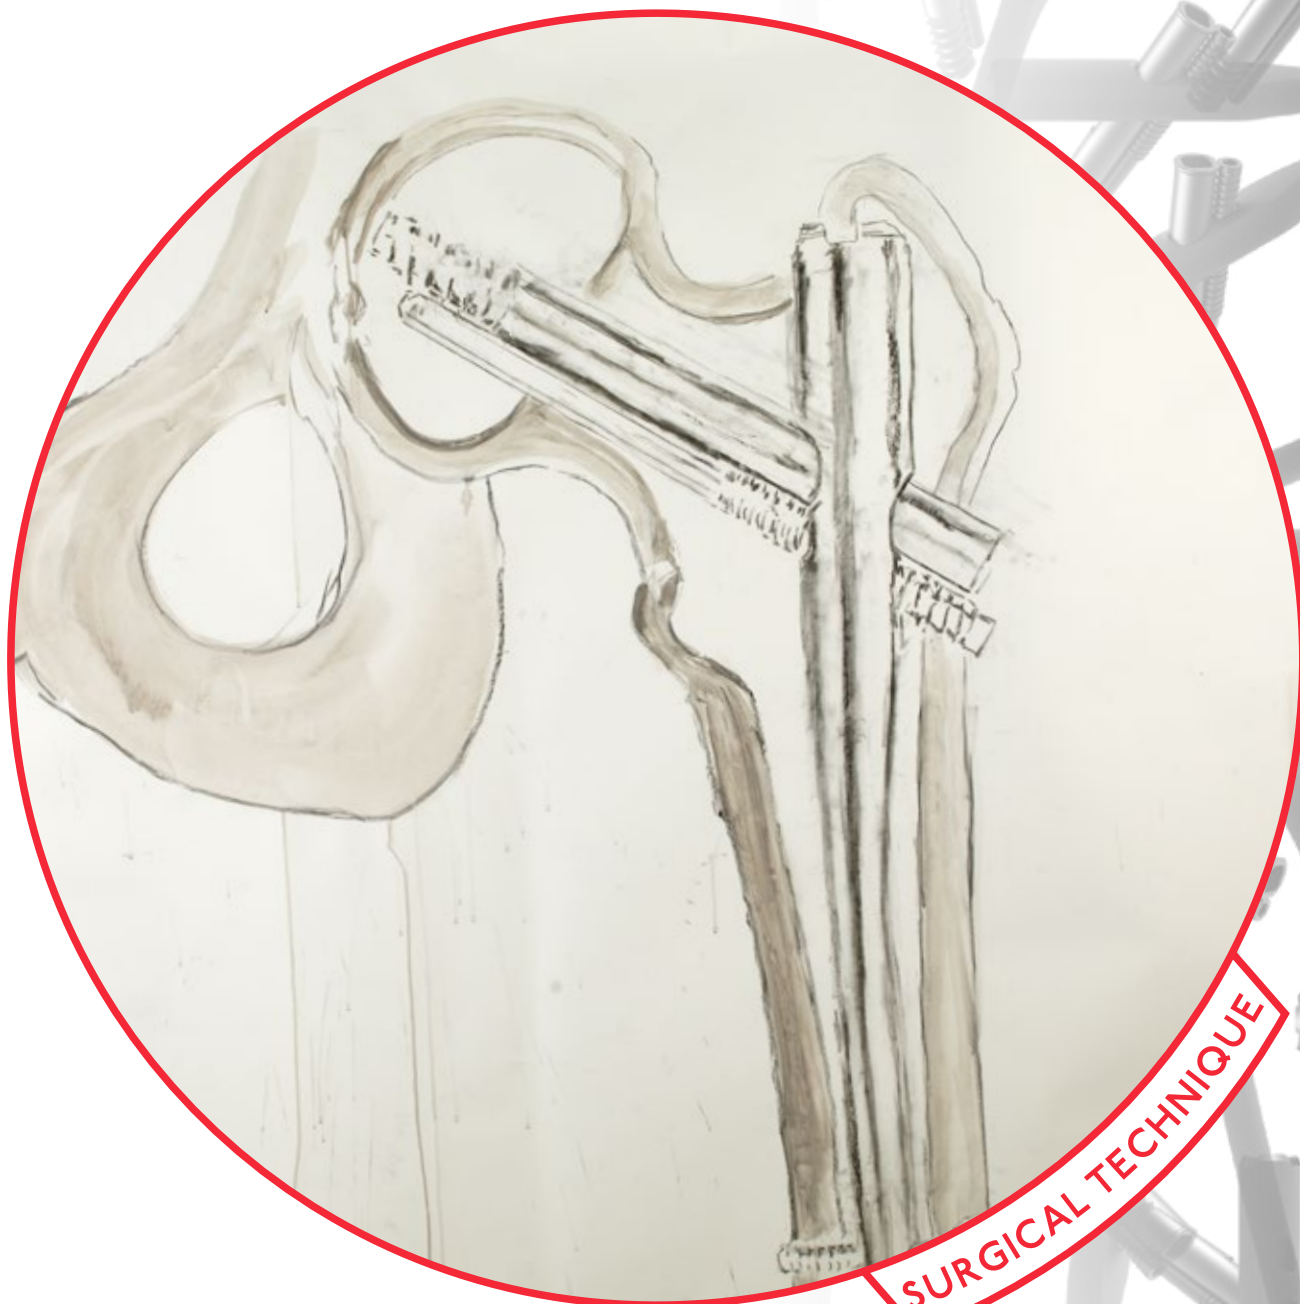

Intramedullary Nailing System

PROXIMAL FEMUR

THE ART of TRAUMA SURGERY

The Art of Trauma Surgery is a collaborative project between I.T.S. and Austrian artist Oskar Stocker that celebrates the skill, perseverance, and artistry of surgeons and engineers who work tirelessly to improve outcomes for trauma patients.

At I.T.S., we stand for long-term, trusting relationships with our customers, suppliers, and development partners. Through our devotion to innovation and development, we continuously seek to improve and optimize products and techniques in the field of traumatology.

We believe that the success of our mission lies in the combination of the technical expertise, compassion and dedication of surgeons and engineers to help patients regain their health and well-being. Join us in celebrating these remarkable individuals and *The Art of Trauma Surgery!*

About the artist

The Austrian artist Oskar Stocker (b. 1956) lives and works in Graz, Austria. He has become known internationally through the exhibition Facing Nations, which consists of portraits of more than 120 people of various nationalities living in Graz; it was shown first in Graz itself, then in Vienna, and later culminated in 2010 with its display at the UN Headquarters in New York City.

In addition to the portraits of individual people, he devotes himself to the depiction of landscapes and objects, down to the smallest detail.





In memoriam

Prof. Dr. Volker Bühren
(*1952 †2023)

Our personal gratitude goes to Prof. Dr. Volker Bühren (Murnau / GER) for guiding this product development from the idea to serial production. His focus has been on reducing clinical problems while improving usability, with the patient and the best possible care always at the heart of his efforts.

His passionate support for all areas of our company were and remain very valuable and will continue to find their way into the product portfolio of I.T.S.

Table of Contents

I. Introduction

8	Background
9	At a Glance
10	Proximale Features
11	Dynamization Control / DyCon®
12	Surgical Technique Overview
14	Nails
16	DyCon® Screw Pair
17	Correction Techniques
18	Closing of Fracture Gap
18	Advanced Compression
19	Indications
19	Contraindications

2. Surgical Technique

22	Diagnostics & Planning
23	Patient Positioning
25	Reduction & Verification of Implant Planning
28	Operative Access to the Trochanter
31	Insertion of the Intramedullary Nail
35	Drill-Wire Positioning
39	Lag Screw Drilling & Insertion
44	Controlled Dynamization: DyCon® Set Screw Drilling & Insertion
47	Guided Distal Locking
50	Disassembly of Targeting Arm
51	Wound Closure & Follow-up
52	OPTIONAL: Correction of Trochanteric Entry Point
54	OPTIONAL: Correction of Lag Screw Drill-Wire
57	OPTIONAL: Closure of a Fracture Gap
58	OPTIONAL: Free Selection of Dynamization Control
60	OPTIONAL: Advanced Compression
62	OPTIONAL: End Cap Screws & Axial Set Screw
63	LONG NAILS: Reduction of the Shaft Fracture &
63	Reaming of the Medullary Canal
66	LONG NAILS: Insertion of the Long Intramedullary Nail
68	LONG NAILS: Free-hand Distal Locking
71	Implant Removal

3. Information

74	Typ II Anodization
75	Article list



Introduction

WARNING: If there is no sufficient bone healing, wrong or incomplete postoperative care, the implant might break.



○ Background


The I.T.S. Intramedullary Nailing System (INS) is based on the proven concepts of intramedullary nail osteosynthesis, first introduced by Küntscher, and integrates the standards established in the following decades across the entire spectrum of intramedullary fracture management. These intramedullary nails and instruments are engineered with the clinical aspects of patient safety as a top priority for the planning, implementation, and follow-up phases.

The INS Proximal Femur nail is designed for the treatment of the full spectrum of fractures, revisions and tumor stabilizations in the area of the proximal femur and also combined forms of injury affecting the shaft area (*for a complete list of indications, see p. 19*). With the patented technology for Controlled Dynamization, built-in precision aides, and intuitive surgical procedure the INS Proximal Femur nail takes major steps in addressing the current shortcomings facing hip fracture nailing today.


The INS Proximal Femur nail features a two-portal concept, maintaining full rotational stability both intra- and post-operatively, with the DyCon® screw pair forming a dynamically controlled force carrier system in the femoral neck and head. Three different neck angles (Centrum-Collum-Diaphyseal [CCD] angles) and a total of 14 nail lengths accommodate variations in patient anatomy. In addition to short and long nails, the system also includes an intermediate nail with distal locking via the targeting module and additional stabilization at the isthmus.

A special focus is placed on geriatric fractures with the goal of immediate postoperative weight-bearing and ensuring optimal biomechanics in the case of osteoporosis.

The top quality of the implants, manufactured in Austria, and the close collaboration with our international expert surgeon design team form the basis of a high-quality and comprehensive global nailing system.

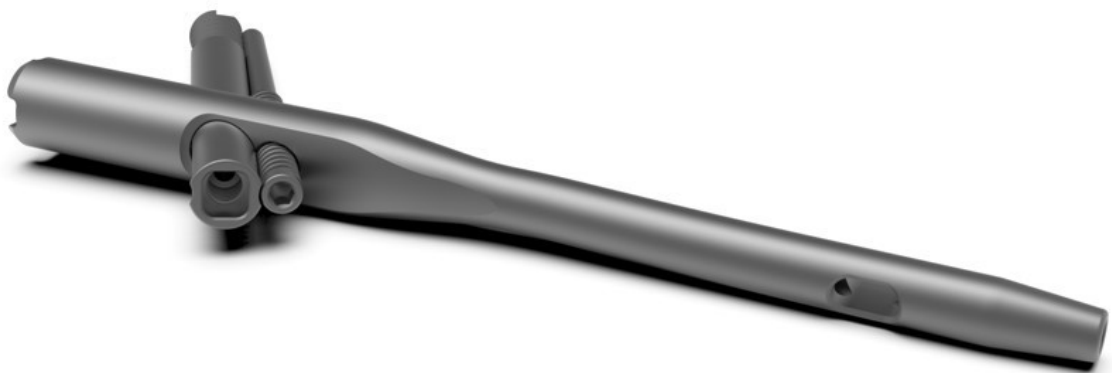

○ At a Glance

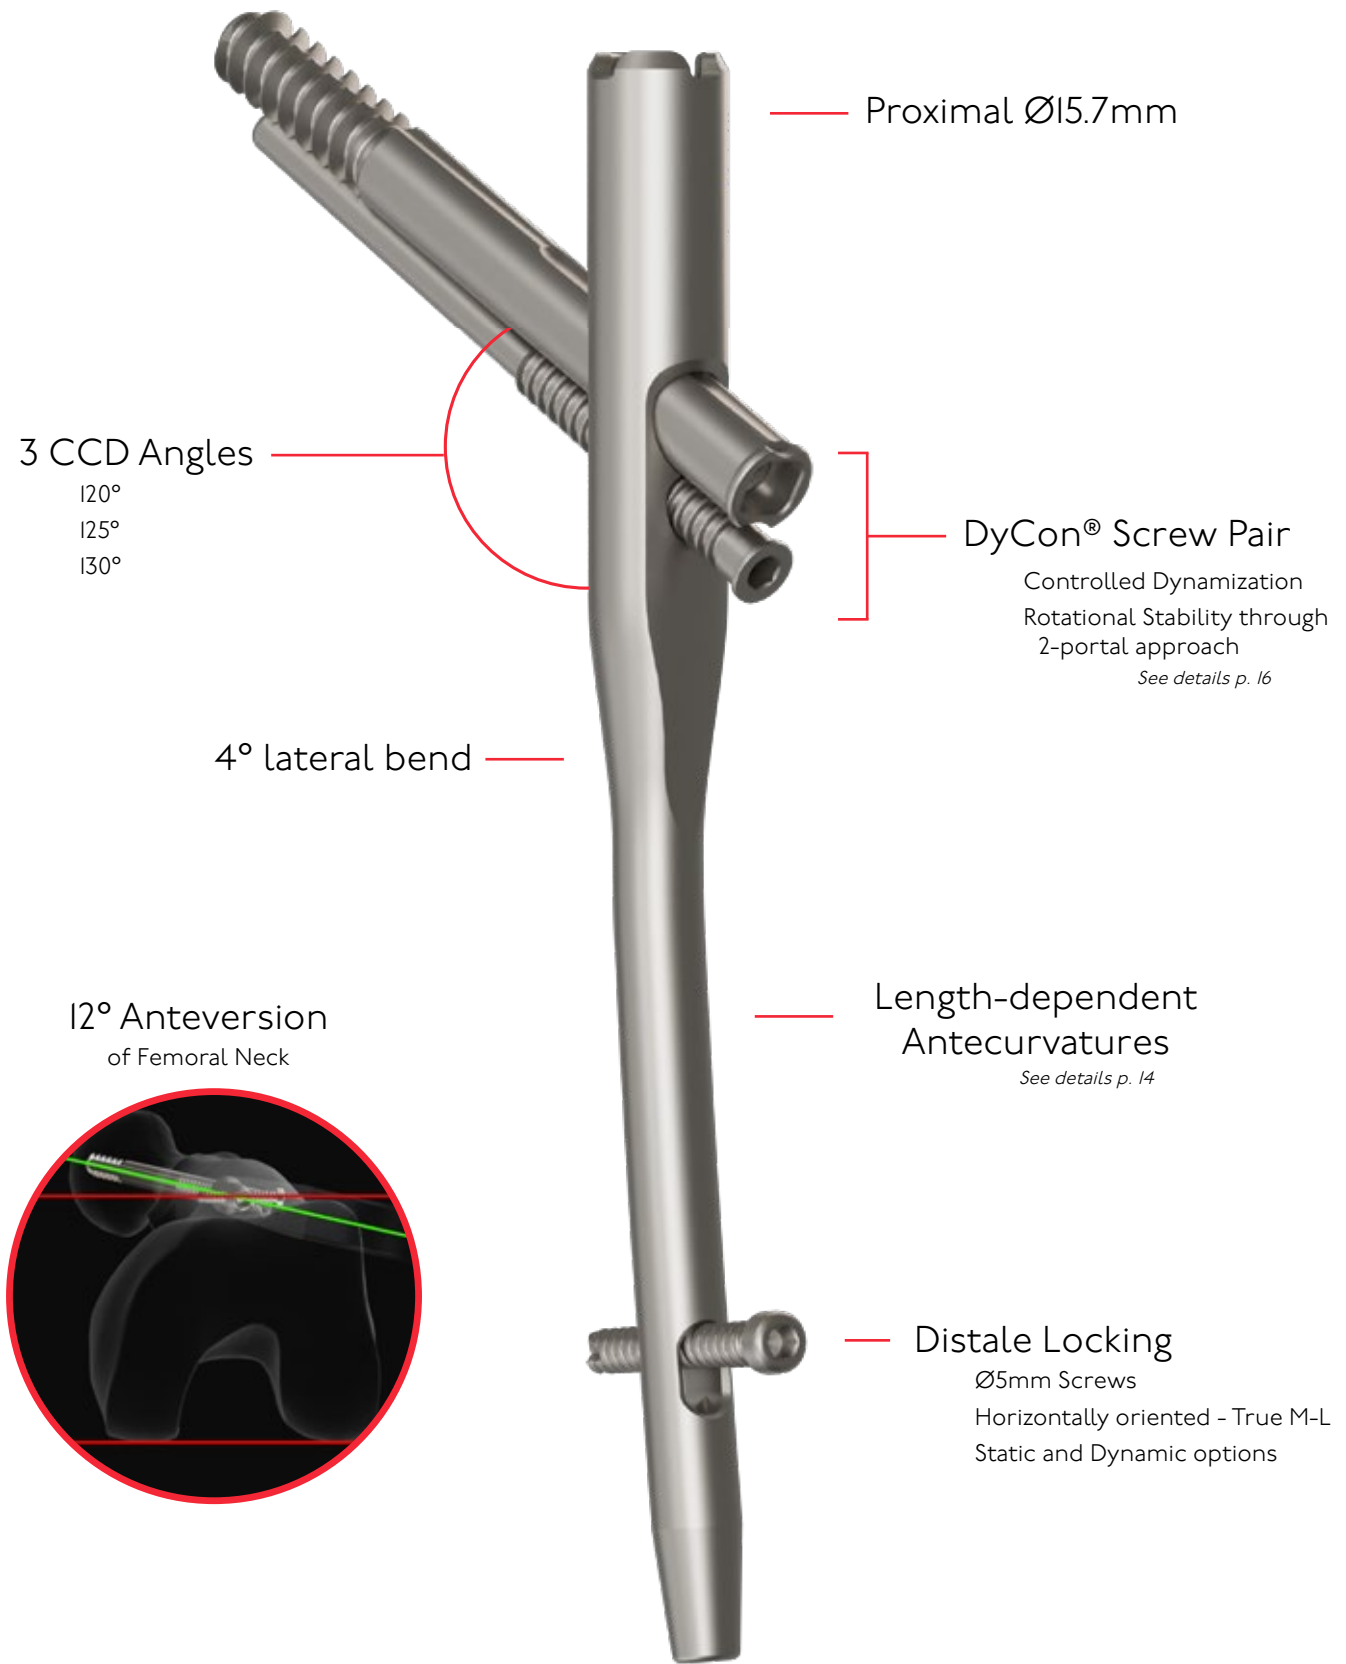

○ Proximale Features

- Easy-to-use, built-in targeting guides to reduce the risk of implant cut-out
- 2 portal approach providing rotational stability both intra- and post-operatively
- Inferior set screw allowing for controlled dynamization
- Built-in closing of the fracture gap and compression of fracture




○ Dynamization Control / DyCon®

The DyCon® Screw pair, consisting of the load-bearing Lag Screw with the inferiorly placed DyCon® Set Screw, forms a dynamically controlled force carrier system in the femoral neck and head.



The inferior DyCon® Set Screw anchors in the nail and runs at a slight angulation into the groove of the Lag Screw. This technology allows for controlled lateral dynamization of the Lag Screw, while inhibiting medial migration with the full contact area between the two screws.

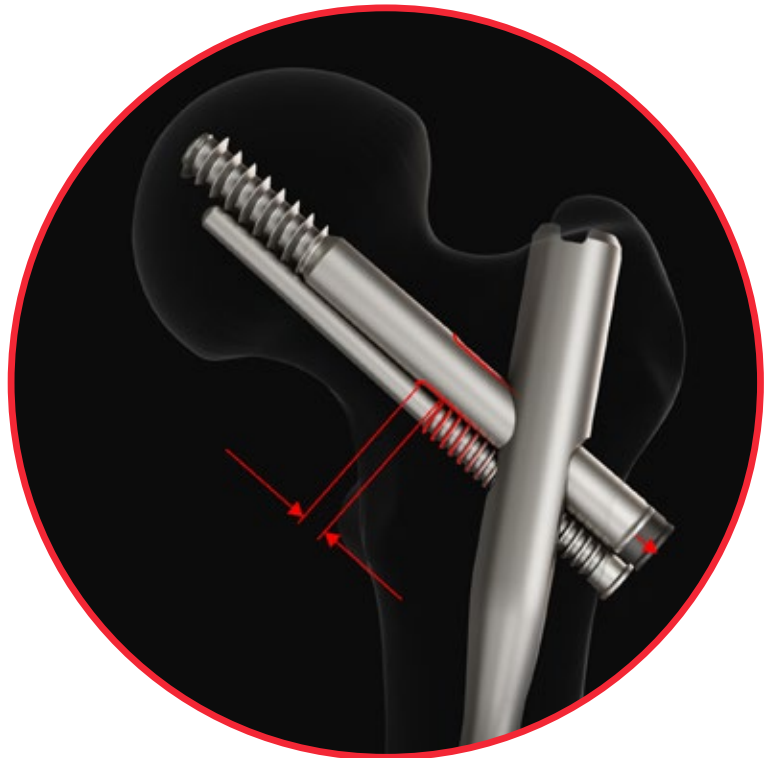

The standard technique describes a recommended 5mm dynamization (*Dynamic mode* - shown above). However, with this design, the lateral movement of the Lag Screw can be controlled in a fully scalable manner, from 0mm (*Static*) to 10mm dynamization (*Dynamic +*).



STATIC




DYNAMIC +

○ Surgical Technique Overview


With the aim of optimizing the flow of surgery and minimizing the risk of user error, the surgical technique for the INS Proximal Femoral Nail follows an intuitive step-by-step working pattern.

For detailed Surgical Technique, see p. 21

Operative Access to the Trochanter

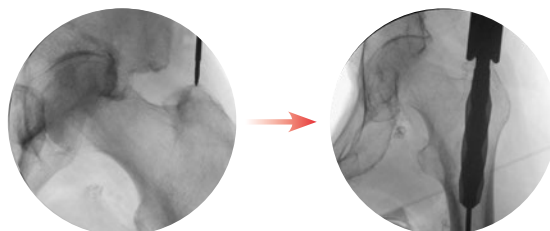


Insertion of the Intramedullary Nail




Drill-wire Placement




Lag Screw Insertion

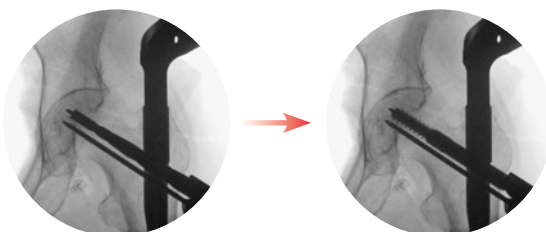


DyCon® Set Screw Insertion

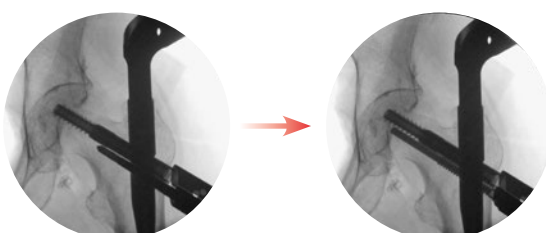


Guided Distal Locking

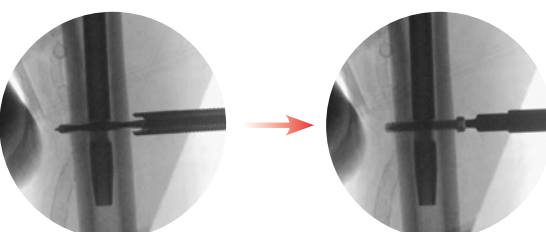

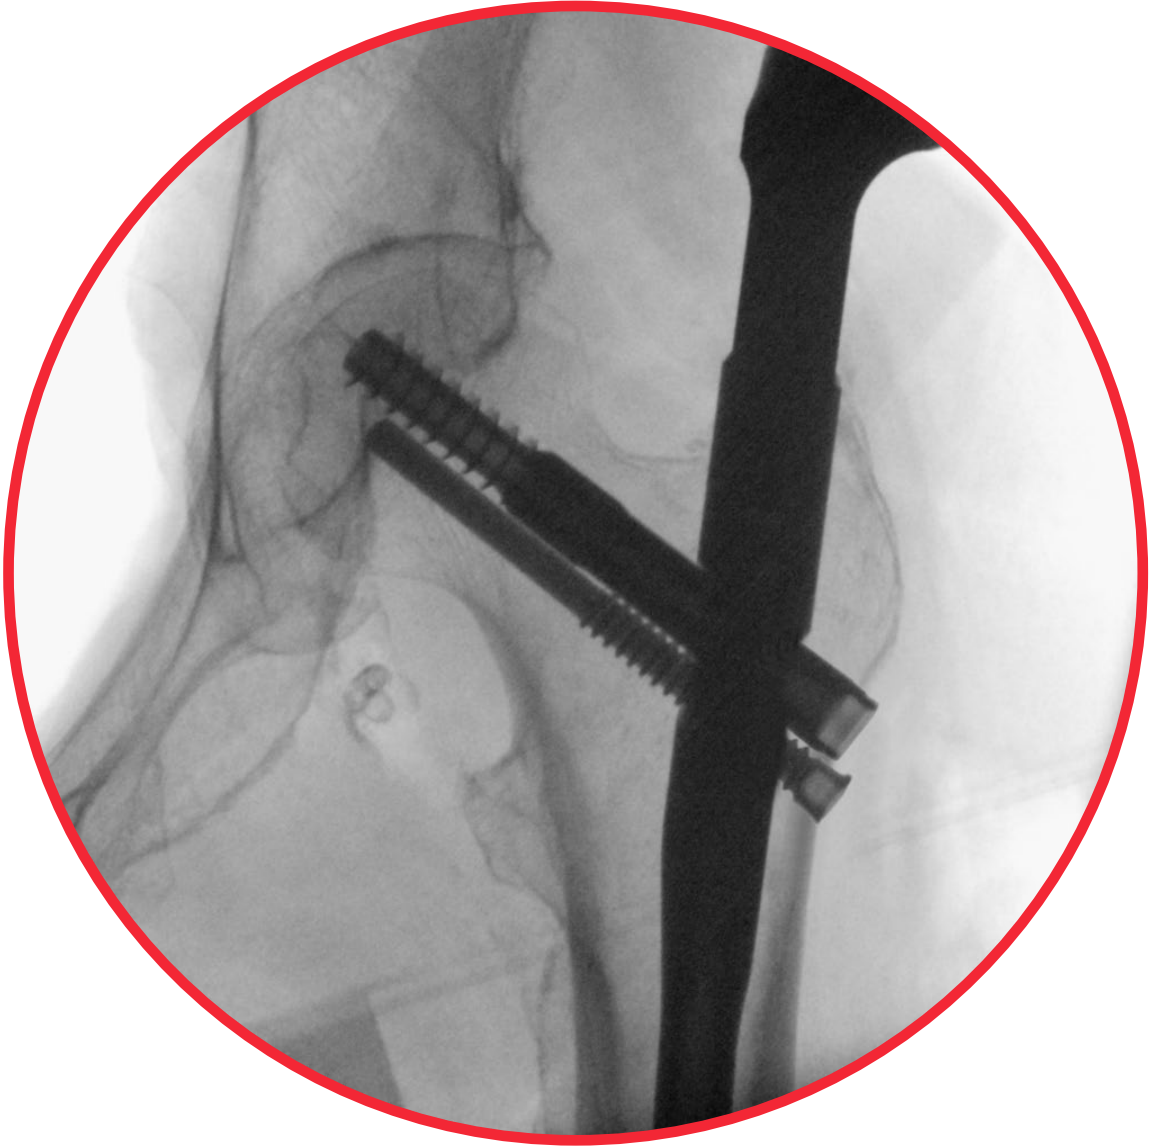


○ Nails

All nails come in left and right versions, with length-dependent antecurvatures to allow for a close anatomical fit to the patient. The short and intermediate nails are indicated for all lengths of femurs and as such use the average femoral antecurvature of 1100mm.

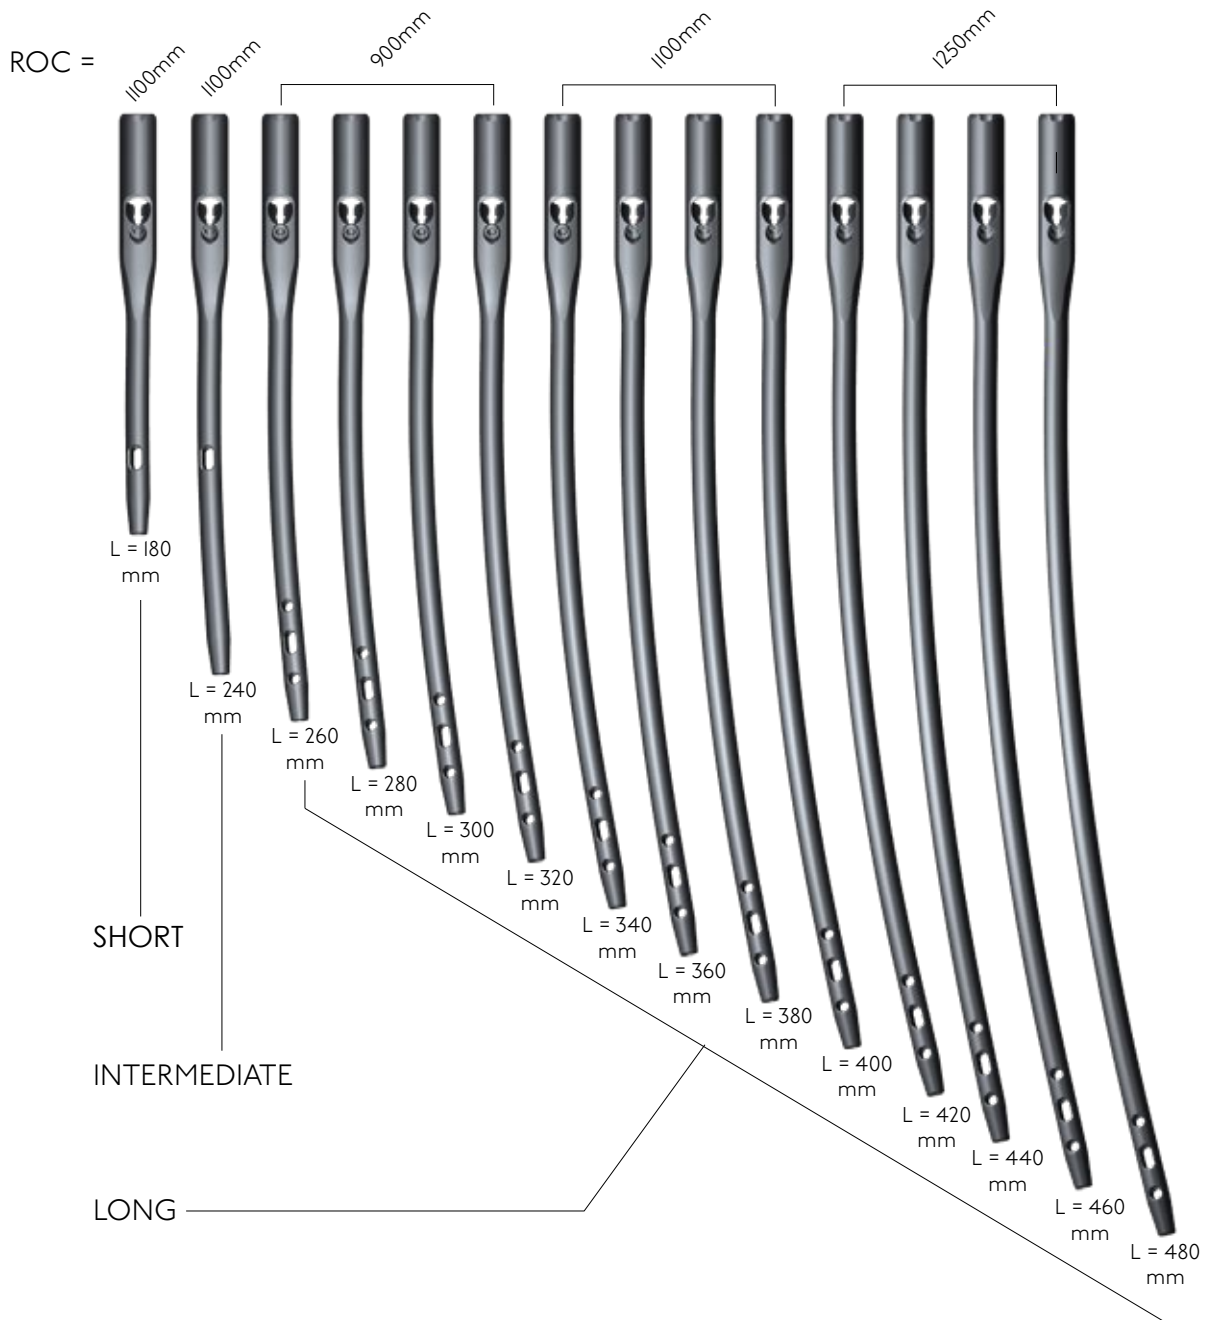

Decision making between the use of intermediate or long nails in highly unstable and more distal subtrochanteric fractures must be individualized. The short version of the nail is intended for stable and moderately unstable pertrochanteric fracture forms. The intermediate version can be used for highly unstable pertrochanteric as well as suitable subtrochanteric fracture forms due to a biomechanically improved support in the femoral shaft, while maintaining the possibility of rapid and easy locking via the target arm. Fractures extending into the shaft as well as combined forms of injury are addressed with the long nails. (For a complete list of indications, see p. 19)

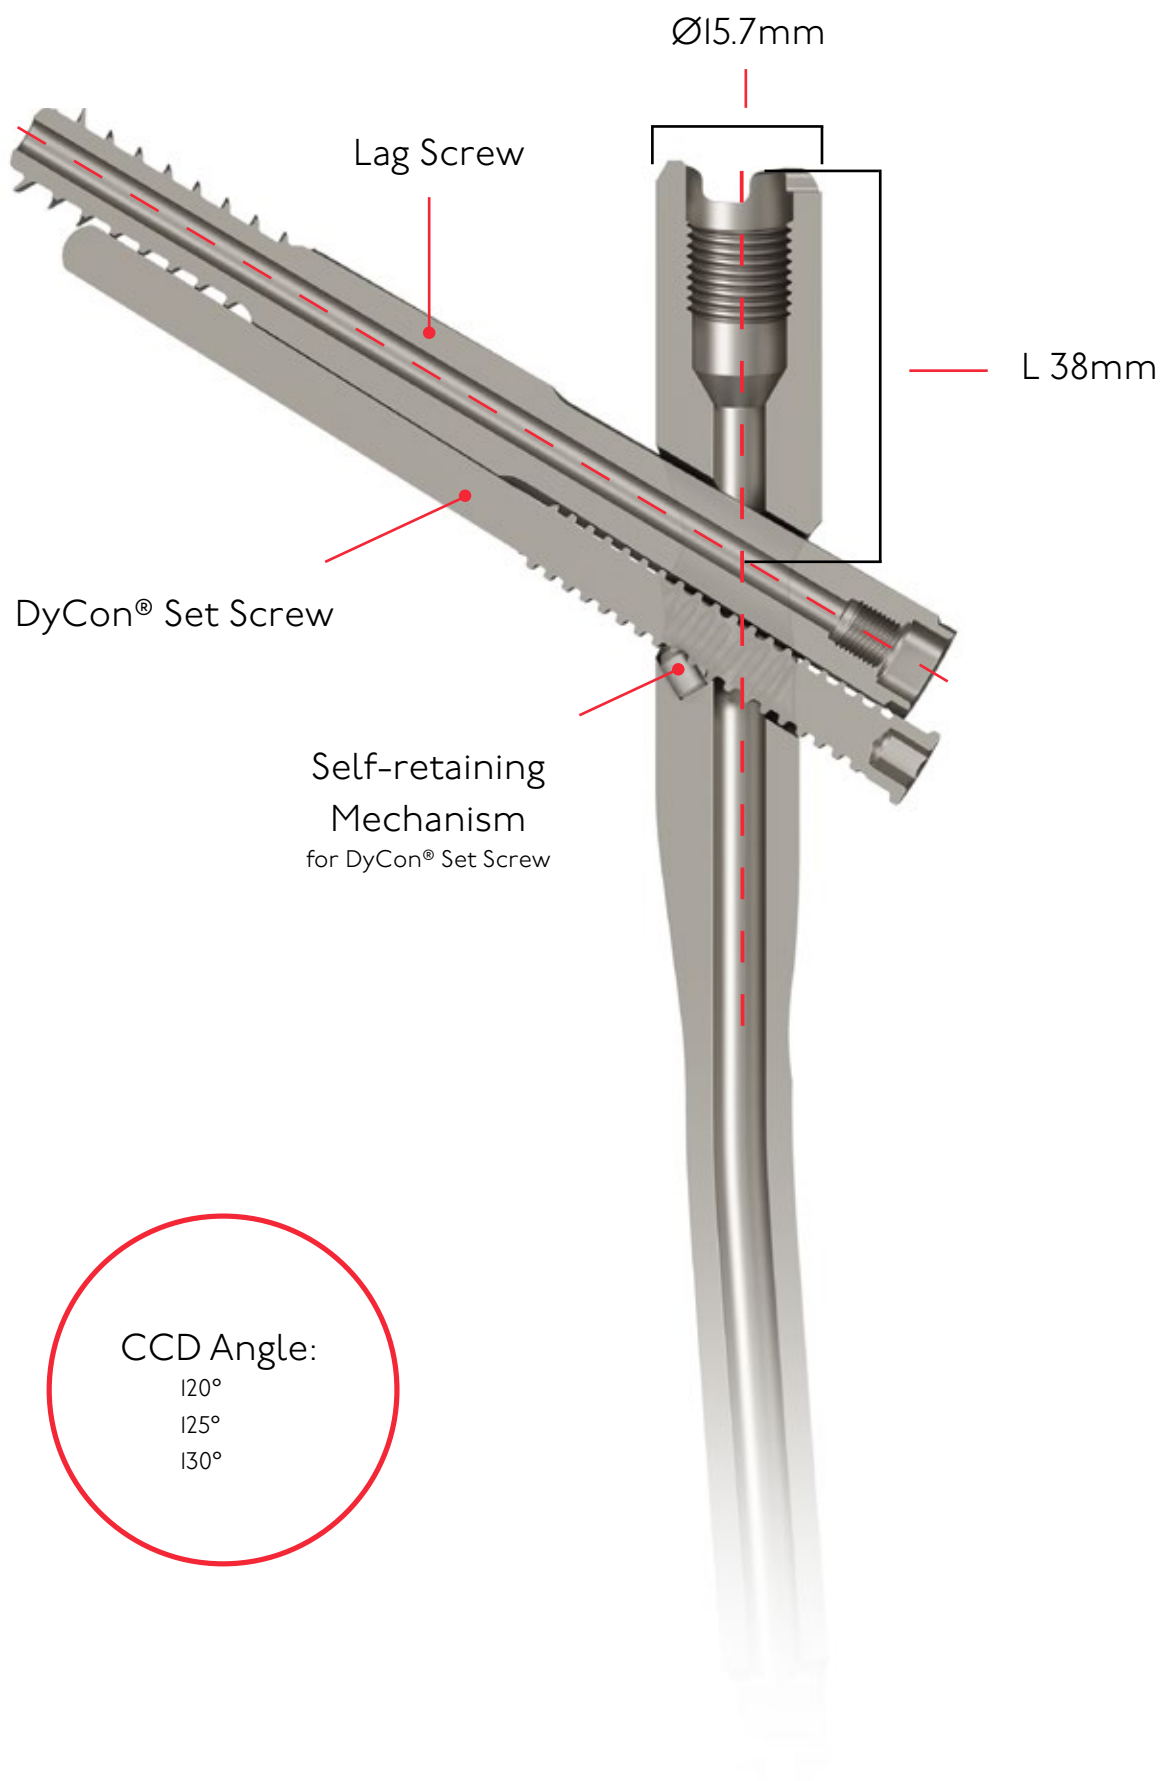

○ DyCon® Screw Pair

The DyCon® screw pair (Lag Screw and DyCon® Set Screw) relies on a 1:1 relationship between the two screws. The DyCon® Set Screw is thus chosen based on the measurement of the Lag Screw. No calculation or conversion is necessary as each DyCon® Set Screw is labeled with the corresponding Lag Screw length to ensure proper function in controlling the amount of dynamization.



Short DyCon® Set Screw

In cases where needed or preferred, a short version of the DyCon® Set Screw is available. The Short DyCon® Set Screw has the same dynamization control function as the standard versions and can be used universally for all lengths.

See technique p. 45




Optional End Cap Screws with Axial Set Screw Function

The optional end caps are designed to include an axial set screw function, and are available with extensions ranging from 0-20mm. The end caps can be used both in the presence or absence of the DyCon® Set Screw.

See technique p. 62

Functions:

- keeps the thread free of scar tissue for a planned implant removal
- extends the proximal nail portion (5 - 20mm)
- provides rotational locking of the Lag Screw in the absence of a DyCon® Set Screw

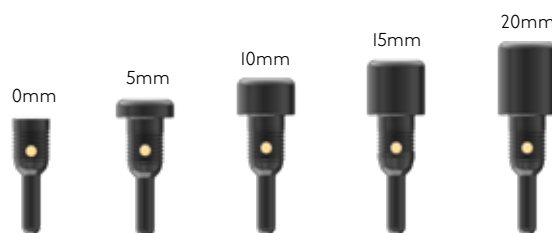

○ Correction Techniques

The INS Proximal Femur includes a number of optional techniques to allow the surgeon to optimize the procedure as needed for each individual patient and surgery.

Rescue Sleeve for Correction of Trochanteric Entry Point

An optional rescue sleeve is available in case of a need to correct the original trochanteric entry point. The rescue sleeve is placed over the opening reamer sleeve and allows trochanteric opening to be adjusted either medially or laterally by a distance of 5, 10 or 15mm.

See technique p. 52



Correction of Lag Screw Drill-wire

The two-portal design allows for a simple, guided correction of the Lag Screw Drill-wire if needed. Thanks to the parallel trajectories of the two drill-wires, it is possible to adjust the drill-wire positioning superiorly or inferiorly, while retaining the correct central position in the lateral projection.

See technique p. 54



○ Closing of Fracture Gap

Closing of Fracture Gap

Optional instruments are available for closing of the fracture gap by using the Lag Screw. The positioning instrument can be used to move the head fragment laterally.

See technique p. 57




○ Advanced Compression

Advanced Compression

Compression to the fracture can be achieved by the Compression Rod together with the optional Set Screwdriver.

See technique p. 60

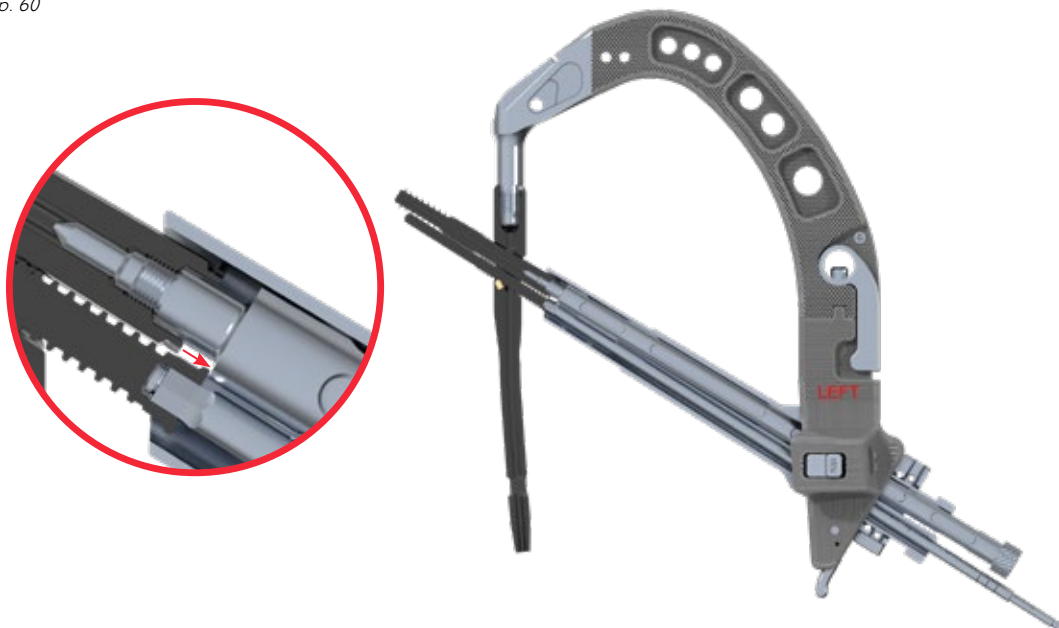

○ Indications

The indications for the I.T.S. Intramedullary Nailing System (INS) - Proximal Femur include intramedullary treatment of fractures and stabilization after tumor resection in the area of the proximal femur, as well as combinations that additionally affect the shaft area using the long nails.

The indications for use of the I.T.S. INS Proximal Femur include:

All Nails:

- Stable and unstable pertrochanteric fractures
- Intertrochanteric fractures
- Combinations of fractures listed above

Additionally for Long Nails:

- Subtrochanteric fractures
- Proximal fractures as listed above associated with shaft fractures
- Pathological fractures in regions as listed above
- Nonunions and malunions in regions as listed above

○ Contraindications

Contraindications generally exist in the case of growth plates that have not yet been fused and in special circumstances such as infection or marked local inflammation.

Before choosing the implant certain precautions regarding preexisting and fracture related conditions have to be taken into account. As for most intramedullary implants, the I.T.S. INS Proximal Femur Nailing System is designed to stabilize fractures temporarily until bony healing occurs and therefore depends on the patient's bone quality for adequate fixation. Conditions such as compromised vascularity, excessive stresses on bone and implant such as severe obesity or degenerative diseases have to be considered as well as every interfering systemic condition such as infection, demonstrated allergy or foreign body sensitivity to any of the implant materials. The decision whether to use the system in these conditions must be made by the physician taking into account risks versus benefits.



Surgical Technique

IMPORTANT: All instruments and implants in this surgical technique are calibrated to each other so that general instruments are not to be used unless specifically named.

2.

○ Diagnostics & Planning

Standardized fracture-related diagnostics for proximal femur fractures consist of a pelvic overview image and longitudinal images of the affected femur with the hip joint in the anteroposterior (a/p) direction and in a lateral projection if feasible due to pain. In the majority of cases, and especially in older patients, these images can be used to plan the procedure and select the appropriate implant. For complex and unclear fracture patterns, and especially for high-energy trauma in younger patients, additional clarification by means of computed tomography with reconstruction may be indicated.

Depending on the type of the fracture, the number of fragments, the dislocation, and other parameters, such as the integrity of the lateral femoral cortex, the fracture is classified as stable, unstable or highly unstable. Special cases are, for example, reverse oblique fractures that are difficult to reduce or fractures that have subtrochanteric extension. Accompanying pathologies beyond the actual fracture situation, such as hip joint arthrosis or tumorous destruction, must also be included in the planning.

For the planning of the implant position, the insertion depth of the Lag Screw, and the rotational locking of the Lag Screw with the alternatives of a long or short DyCon® Set Screw, the degree of pre-existing osteoporosis is an essential consideration. This should be evaluated both for the femoral head with the typical structural weakening, and for the shaft area with a typical thinning of the femoral cortex, e.g. indicating the use of the intermediate nail.

For prior planning of the implant configuration of the nail and Lag Screw, a mirror image of the opposite side is helpful. Essential factors are the femoral neck - diaphyseal angle and the width of the femoral medullary canal. The angle can be determined preoperatively analogously with a surgical goniometer or digitally in the X-ray PACS, whereby various software solutions also allow planning with projection of the implants. Essential for the selection of the nail diameter is the analysis of the femoral medullary canal width, especially in the isthmus region, under projection of the planned nail position.

Usually, an end position of the Lag Screw thread centrally in the femoral head is aimed for. For the application of the DyCon® Set Screw, it is necessary to maintain a sufficient distance between the Lag Screw and the cortex of the Adam's arch at the femoral neck for the passage of the DyCon® Set Screw. In case of an inferior implantation of the Lag Screw close to the Adam's arch, the use of a short DyCon® Set Screw should be considered.

○ Patient Positioning

- The patient is placed in the supine position on an operating table with unobstructed fluoroscopy and freely adjustable extension device via a foot fixation.

ALTERNATIVE: It is also possible to treat the patient in the lateral position (e.g. in the case of shaft fractures), whereby a more difficult reduction of the proximal fracture must also be taken into account.

- The arm of the affected side is attached to a splint across the body.

TIP: If possible, the upper body is angled slightly by about 15° to the opposite side.

- The healthy leg is also rotated as far as possible to the opposite side with 90° flexion of hip and knee with the lower leg on a padded support.

TIP: To support reduction under traction, a padded post is positioned inguinally on the inner side of the affected thigh.

- The image intensifier is placed between the legs from the foot end. The aim is to obtain two standard projections of the hip joint with the adjacent femur by rotating the C-arm 90° under the leg to be operated on.

TIP: In the a/p position, the femoral head with acetabulum, the femoral neck and 10 to 15cm of the proximal femur with the trochanteric mass should ideally be imaged.



- The lateral projection is adjusted in relation to the femoral neck angle (e.g., at 120° by 30° or at 130° by 40°) rotated to the longitudinal body axis in order to obtain a projection of the femoral neck in the lateral plane.



CCD	Einstellung des Projektionswinkels
120°	30°
125°	35°
130°	40°

○ Reduction & Verification of Implant Planning



The aim is to achieve a closed reduction of the main fragments, i.e. for the femoral shaft versus the proximal fracture portion with femoral neck and femoral head in terms of length, axis and rotation.

NOTE: Accurate reduction of the fracture before nail insertion is the first mandatory key point to achieving a satisfactory outcome.

TIP: If satisfactory reduction cannot be achieved closed, assisted percutaneous techniques can be used during surgery. If a complex fracture is irreducible closed, which is more often the case with e.g. displaced subtrochanteric fractures, an open reduction technique should be used.

IMPORTANT: Drill-wires are single use instruments and must not be reused.

- First, reduction is performed by increasing traction under image intensifier control in the a/p projection. The traction should bring the leg into a horizontal position corresponding to the condylar axis of the femur parallel to the body axis without distracting the fracture.

TIP: In highly unstable fracture patterns, it may be helpful to mount an additional support for the proximal femoral region from below the table.

- Next, the reduction is checked by pivoting the image intensifier to the lateral position.
- Readjustments are to be made first by rotating the leg usually inward or otherwise outward.

TIP: An initial check of correct rotation can be made visually by looking at the position of the patella compared to the position of the femoral neck using fluoroscopy. With the patella in a horizontal position corresponding to a neutral femoral condyle axis parallel to the floor, the neck of the femur should move upward 10-15° in the image intensifier image or anterior to the projection in the anatomic view. Alternatively, inward rotation of the patella by 10-15 deg can be performed and with the fracture satisfactorily reduced, a perfect lateral of the femoral neck should be seen.


- The cover should leave a surgical field 20cm wide on the lateral thigh, with the center of the surgical field above the palpable greater trochanter. Cranially, the surgical field begins above the iliac spine; caudally, the area for the short and intermediate nails extends to the middle of the thigh; for the long nail, below the knee.

TIP: The surgical field should be taped off as fixation of the drapes with clamps may obscure fluoroscopic imagery.


- Fluoroscopy in the a/p projection in the reduced state can now be used to check the planning of the implant selection and in particular the selection of the femoral neck-diaphyseal angle. The x-ray ruler (*PF X-Ray Ruler, Short or PF X-Ray Ruler, Long for the long nails*) allows measurement of the CCD angle (together with an inserted drill-wire (*Precision Drill-Wire, Ø3.2x390mm*) as well as planning for the nail length, whereby the anticipated location of the distal locking can be estimated.

TIP: The indicator window at the proximal end of the x-ray ruler (*PF X-Ray Ruler, Short or PF X-Ray Ruler, Long for the long nails*) shows the path of the guiding drill wire during the proximal access to the trochanter.

NOTE/CAUTION: By placing the x-ray ruler in the a/p projection using the image intensifier, the medullary canal width and thus the required nail diameter can also be estimated. However, for the calculation, it must be taken into account that, depending on the distance between the x-ray ruler and the bony femur, a projection effect occurs due to the soft tissues in between. With a radiation source located at a distance of 5 to 10cm above the leg, this causes an increase in the reading of 2 to 3mm compared to the actual medullary diameter.

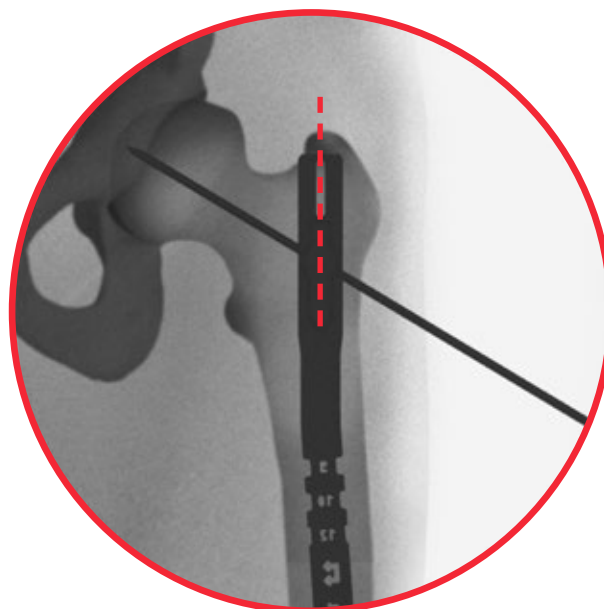


Operative Access to the Trochanter

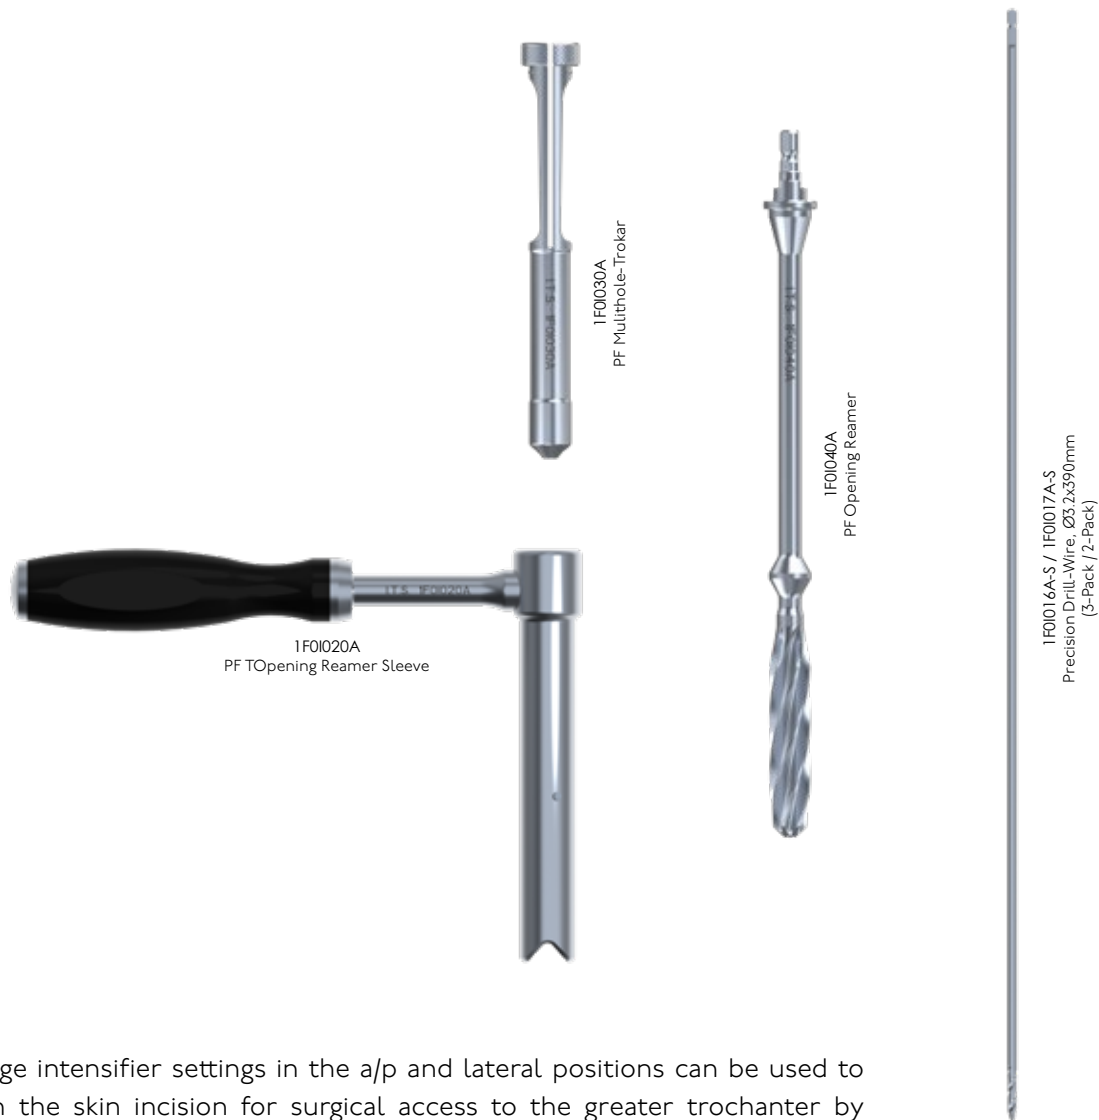

The image intensifier settings in the a/p and lateral positions can be used to pre-plan the skin incision for surgical access to the greater trochanter by placing a drill-wire.


IMPORTANT: Drill-wires are single use instruments and must not be reused.

- In the a/p position, a drill-wire is placed transverse to the body axis so that it comes to rest on the tip of the trochanter in the projection. This height is marked transversely on the lateral thigh.
- In the lateral position of the image intensifier, the drill-wire is placed centrally in the axis of the femur and a mark is drawn longitudinally above the horizontal line.

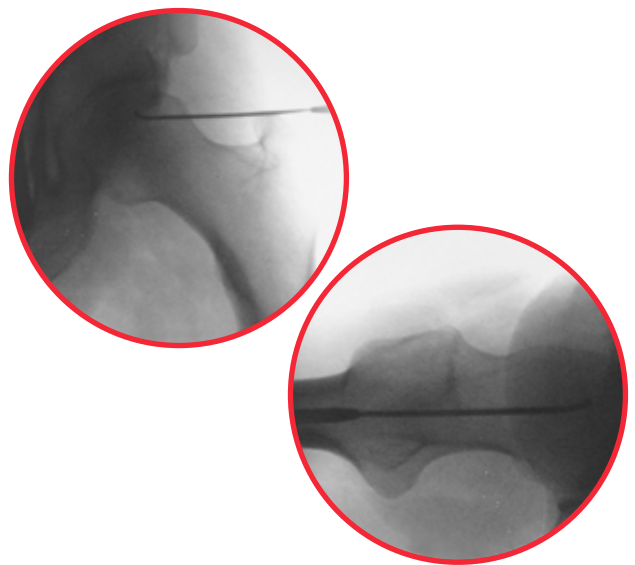

- The skin incision (approx. 2 to 3cm) extends from 2 to 4cm (one to two transverse fingers) proximal to the palpated trochanteric apex or the trochanteric apex defined under radiological control, depending on the amount of the soft tissue.
- After transection of the subcutaneous tissue, the fascia is sharply cut longitudinally. The underlying musculature is elevated until the ridge of the trochanter running from anterior to posterior can be palpated.


- The palpable bone ridge is divided visually into thirds, whereby the correct entry point for the guide wire is usually at the junction of the anterior third and the middle third.

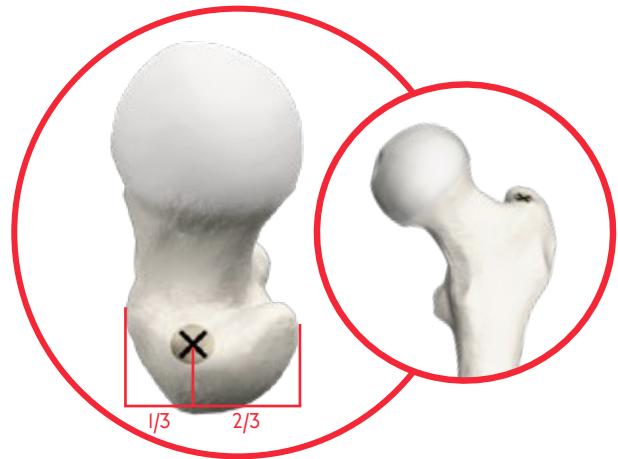

- The guiding drill-wire (*Precision Drill-Wire, Ø3.2x390mm*) is drilled centrally in the longitudinal axis of the femoral shaft, if necessary with the aid of the conical drill sleeve (*PF Multihole Trocar*) with soft-tissue protective sleeve (*PF Opening Reamer Sleeve*) and under image intensifier control, whereby the valgus path must be observed in the a/p projection.


IMPORTANT: The correct position of the drill-wire is essential for the following surgical steps and should be implemented and checked with particular care.

TIP: If corrections are necessary, the first drill-wire can be left in place and a second parallel drill-wire can be inserted via the parallel holes of the conical drill sleeve or, alternatively, after appropriate repositioning within the specified hole selection.

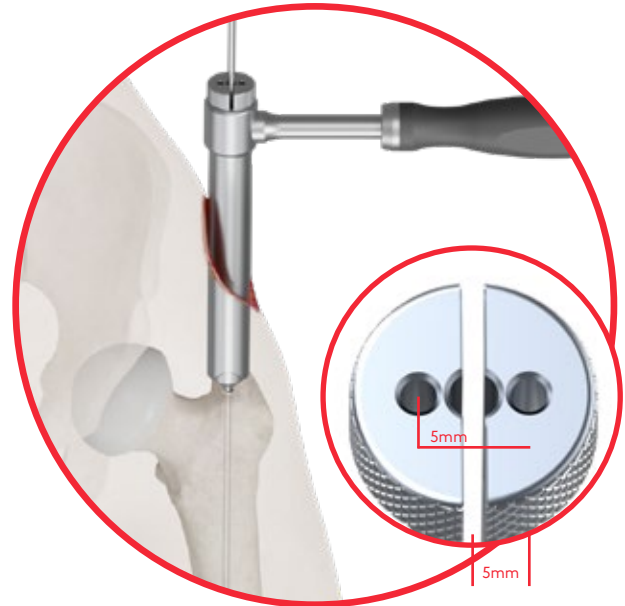

- The conical drill sleeve is then removed, and the soft tissue protection sleeve is advanced so that the dovetail-like shape sits laterally and medially over the trochanteric ridge.
- The medullary canal is then opened over the drill-wire with the opening reamer through the soft tissue protection sleeve until the depth stop makes contact with the tissue protection sleeve.

IMPORTANT: All reaming steps should be performed under image intensifier control.

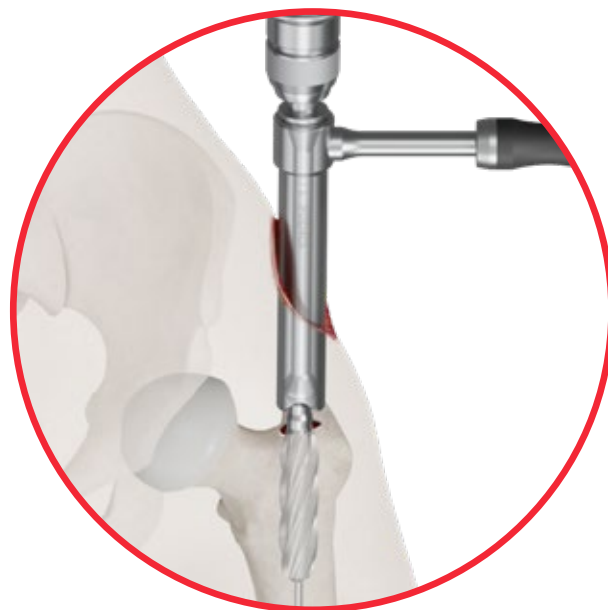


TIP: If the drilled opening is too medial or lateral, the rescue sleeve (*PF Opening Reamer Sleeve Rescue*) can be used, see p. 52.

For the short and intermediate nail, the opening procedure is thus completed and the instruments can be removed.

TIP: As an option if the medullary canal appears very narrow, the ball tip guide wire (*Ball Tip Guide Wire, Ø3x800mm*) is inserted through the soft tissue protective sleeve and the medullary canal is reamed over the wire.

The continued procedure when using the long intramedullary nails is described separately - see p. 63.

○ Insertion of the Intramedullary Nail

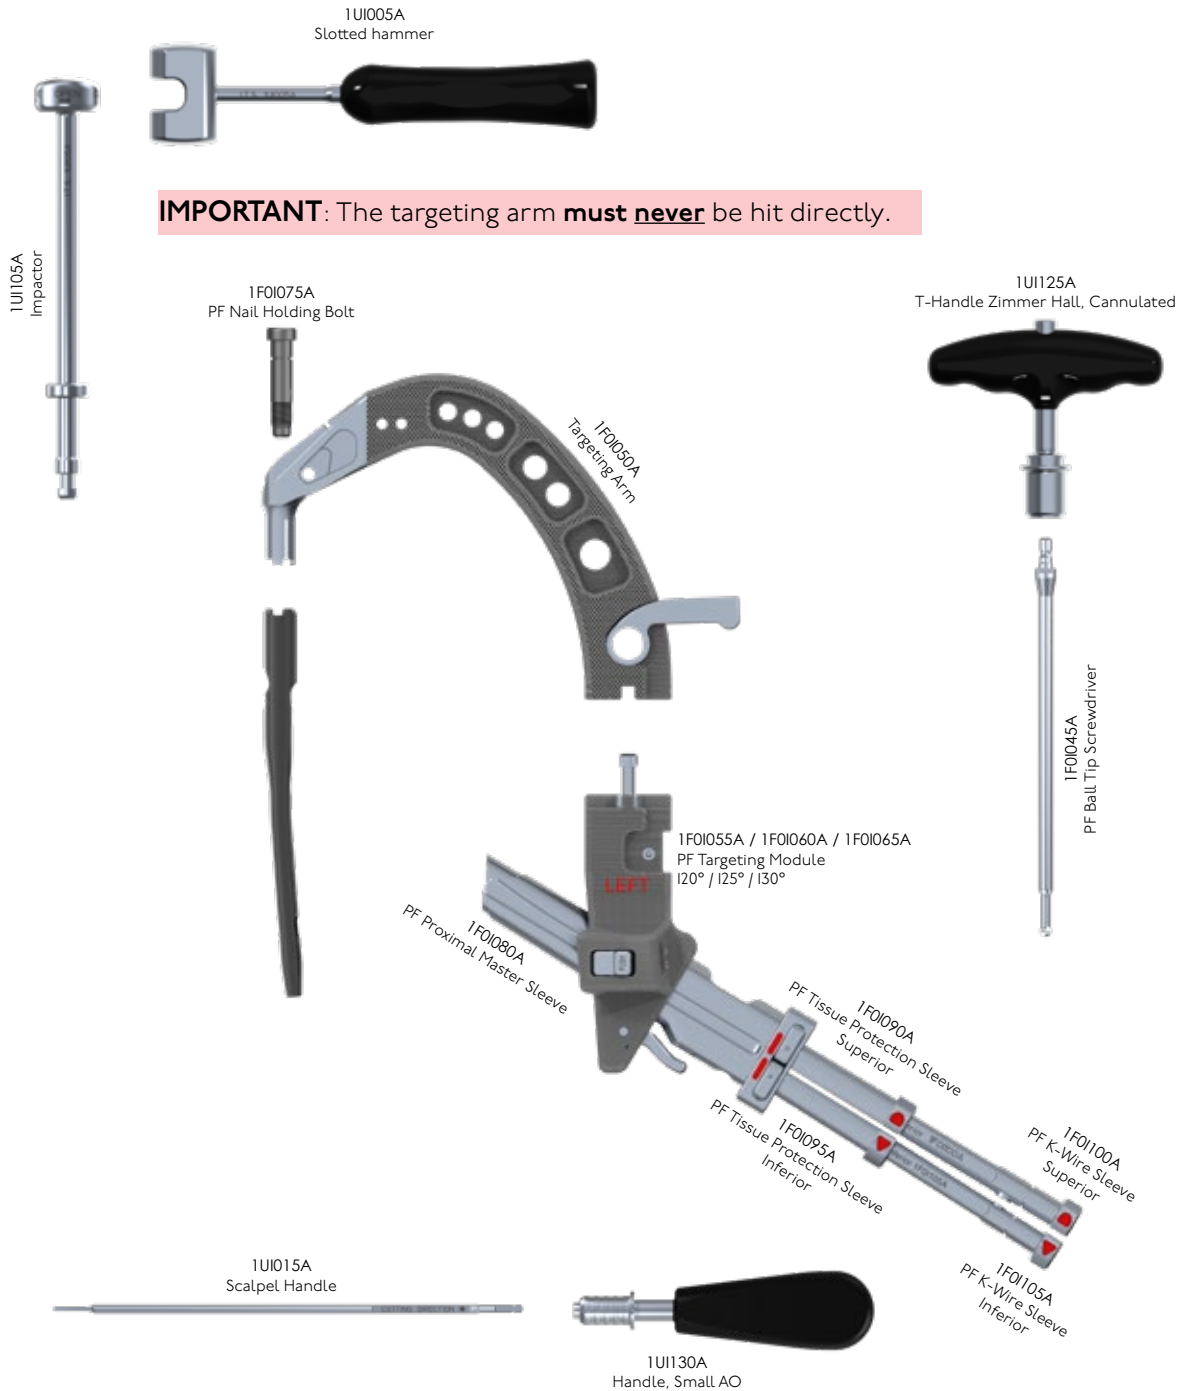

Insertion of the Intramedullary Nail

COLOR CODING

Adhering to the navigation principles of Right/Starboard = **GREEN** and Left/Port = **RED**, the INS system is color coded for easy identification. The targeting module as well as all sleeves are clearly marked indicating their correct orientation.



- The medullary nail is selected with regard to length, femoral neck angle and diameter.
- The nail is attached to the targeting arm by the nail holding bolt which is inserted using a ball-tip screwdriver (*Targeting Arm with Locking Lever, PF Nail Holding Bolt, PF Ball Tip Screwdriver incl. T-Handle Zimmer Hall Cannulated*).

IMPORTANT: The targeting module (*PF Targeting Module 120°, 125° or 130°*) must be double-checked for compatibility with the femoral neck angle of the mounted nail.


IMPORTANT: The retaining screw (*PF Nail Holding Bolt*) securing the nail must be fully tightened to ensure that the nail does not loosen during insertion.

- The intramedullary nail is inserted into the entrance of the canal and advanced with a slightly rotating movement.

ALTERNATIVE: The intramedullary nail can be inserted over a ball-tip guide wire.


TIP: By lifting the insertion handle with resulting inward rotation, the antecurvature of the nail can be used to support the valgus entry path, if necessary, in contact with the medial cortex.

IMPORTANT: After the insertion of the nail, revalidate the attachment of the retaining screw (*PF Nail Holding Bolt*) to the nail to ensure it is secure.

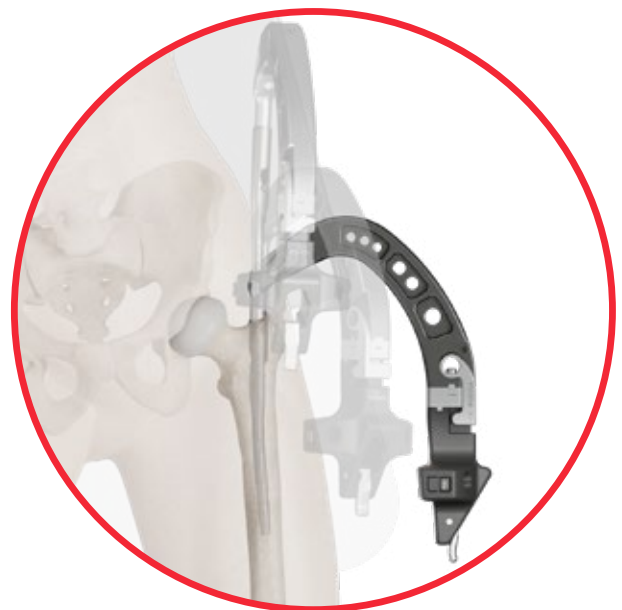


- The implantation depth is indicated by the hole configuration for the femoral neck screw seen in the image intensifier.

TIP: When the leg has ideally been aligned horizontally with respect to the condylar axis, the insertion handle should be rotated towards the floor according to the anteversion of the femoral neck. If the leg has been turned inward - or more rarely outward - and fixed during reduction, the insertion handle must be adjusted accordingly.

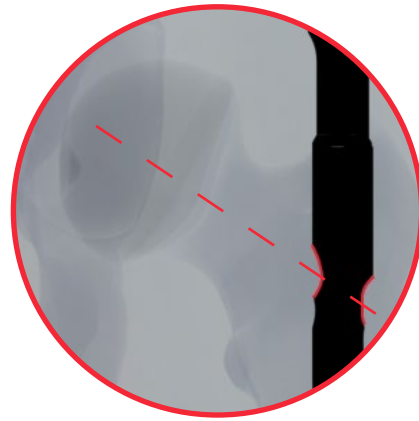

- The soft tissue access (approx. 35mm incision) for positioning the femoral neck implants is started through the Master Sleeve opening in the Targeting Module using a scalpel (*Scalpel Handle*). It is then continued through the subcutaneous tissue and fascia until the bone is reached.

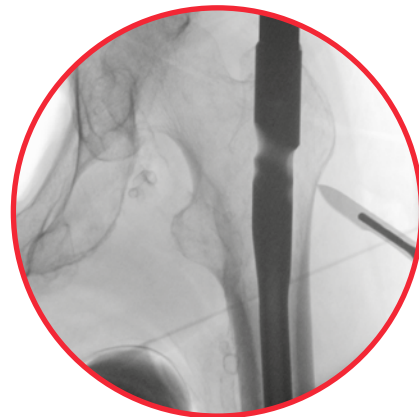

- The Master Sleeve (*PF Proximal Master Sleeve*) is then inserted into the corresponding hole in the Targeting Module and locked in place by turning the locking lever downwards.



- The K-wire Sleeves (*PF K-Wire Sleeve, Superior & Inferior*) are inserted into the corresponding Soft Tissue Protection Sleeves (*PF Tissue Protection Sleeve, Superior & Inferior*), and inserted fully into the Master Sleeve until contact with the lateral femoral cortex is made.

IMPORTANT: The Tissue Protection Sleeves must make contact with the lateral femoral cortex. The sleeves are firmly fixed by a ratchet mechanism ensuring correct length measurement in the subsequent surgical steps.

- The nail position is then adjusted using the a/p projection with respect to the implantation height in the femoral medullary cavity.

IMPORTANT: The targeting arm **must never** be hit directly. The impactor must be used in these cases.


TIP: If the nail is firmly seated, fine positioning can be achieved by **light** hammer blows. For this purpose, the impactor (*Impactor*) must be mounted in advance, which then also permits recoil.

IMPORTANT: If rigid resistance is encountered during insertion, the nail must be retracted and the medullary canal reamed accordingly using the ball tip guide wire.

TIP: The soft tissue protection sleeves each contain a line of holes, which when seen in the a/p projection can be used as a guide to visualize the path of the drill-wires.



○ Drill-Wire Positioning

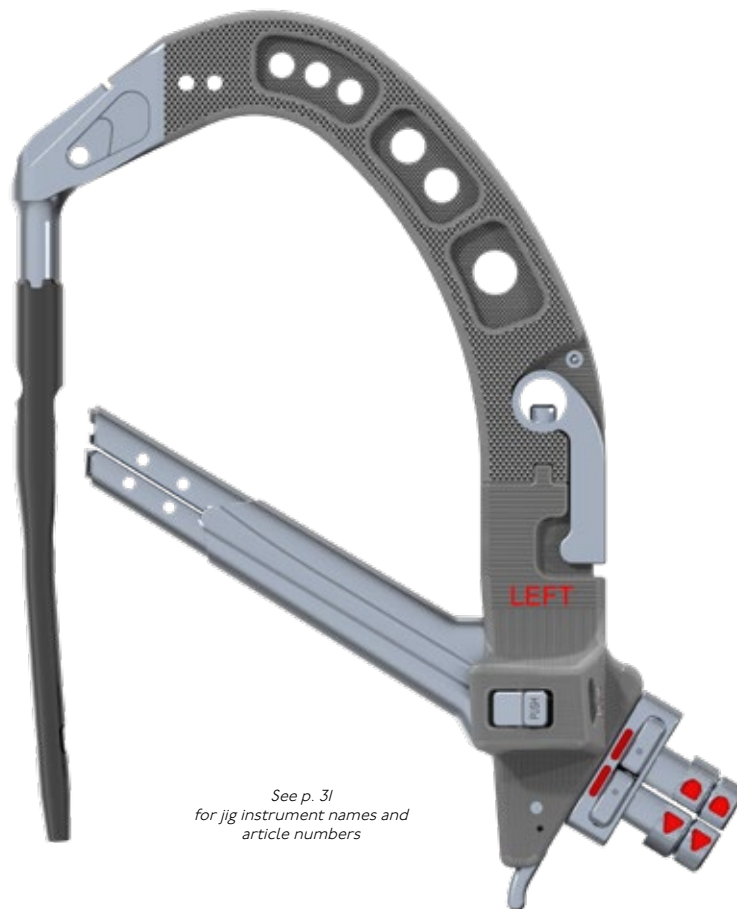

See p. 31
for jig instrument names and
article numbers



1F0I025A
K-Wire Adapter



1F0I016A-S / 1F0I017A-S
Precision Drill-Wire, Ø3.2x390mm
(3-Pack / 2-Pack)


IMPORTANT: Drill-wires are single use instruments and must not be reused.

TIP: For all steps with the drill-wires, the K-wire adapter (*K-Wire Adapter*) should be used, which simplifies the connection to the drill and avoids interference between the wires and power tools with wire driver.

Positioning of Lag Screw Drill-wire:

- Once the desired nail position has been achieved, the image intensifier is rotated into the lateral projection of the femoral neck so that the femoral head appears in a central position.

TIP: The optimal position of the image intensifier is in the approximate lateral projection of the femoral neck. A reception hole in the targeting device allows for the placement of a drill-wire to indicate the direction of the image intensifier.

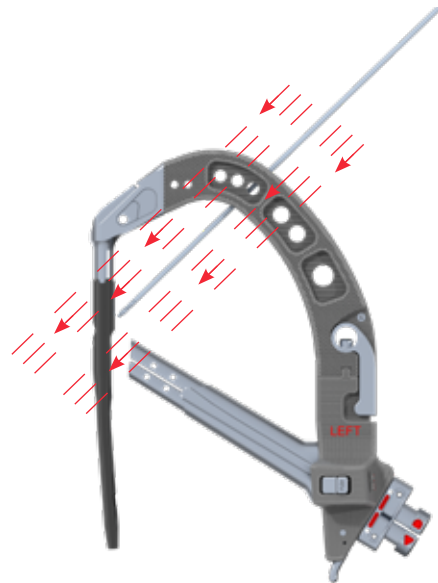


- By slightly rotating the nail, the integrated sighting device on the targeting arm can be centrally adjusted to the center of the femoral head.

IMPORTANT: Before proceeding, ensure that no drill-wire or Guide Wire used in earlier steps remains in the canal/nail.

- In this position, the drill-wire of the Lag Screw is drilled through the superior K-wire sleeve to a central position in the femoral head. This procedure initially fixes the nail and targeting device in a correct lateral position to the femoral neck and femoral head.

IMPORTANT: To avoid perforation into the joint, the drill-wire should never be predrilled too far medially in this initial placement step.

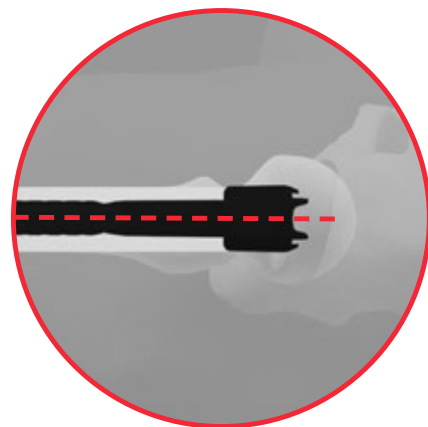

The image intensifier is then returned to the a/p position and the guide wire position is checked.

- If the position in the femoral head corresponds with the original plan, the drill wire for the Lag Screw can be definitively positioned in the a/p projection. The final position of the drill wire tip should be 5mm below the transition of the bony zone into the cartilage of the femoral head, depending on the bone quality and surgeon preference.

IMPORTANT: Make sure that drill-wires are straight and have an undamaged surface to guarantee the safe function with instruments and implants in subsequent steps.

TIP: If the position of the drill-wire is not in the correct position in the femoral head, the position can be corrected both superior or inferior using the parallelity of the two drill-wire trajectories. See p. 54



Positioning of DyCon® Set Screw Wire:

- The inferior drill-wire is placed through the corresponding K-wire sleeve.



TIP: As a rule, this is anchored in the femoral head with a 5 to 10mm shorter length than the Lag Screw drill-wire.



IMPORTANT: The drill-wires are inserted in true parallel paths in order to provide clear visualization that the drill-wires have not been deflected, e.g. by the cortical bone in the Adam's Arc. Should a deflection be observed, the inferior drill-wire should be backed out to a point prior to the deflection. In such cases, only a short DyCon® Set Screw can be used.



○ Lag Screw Drilling & Insertion

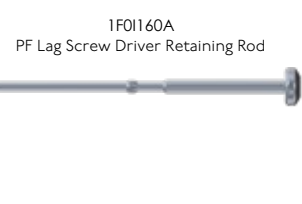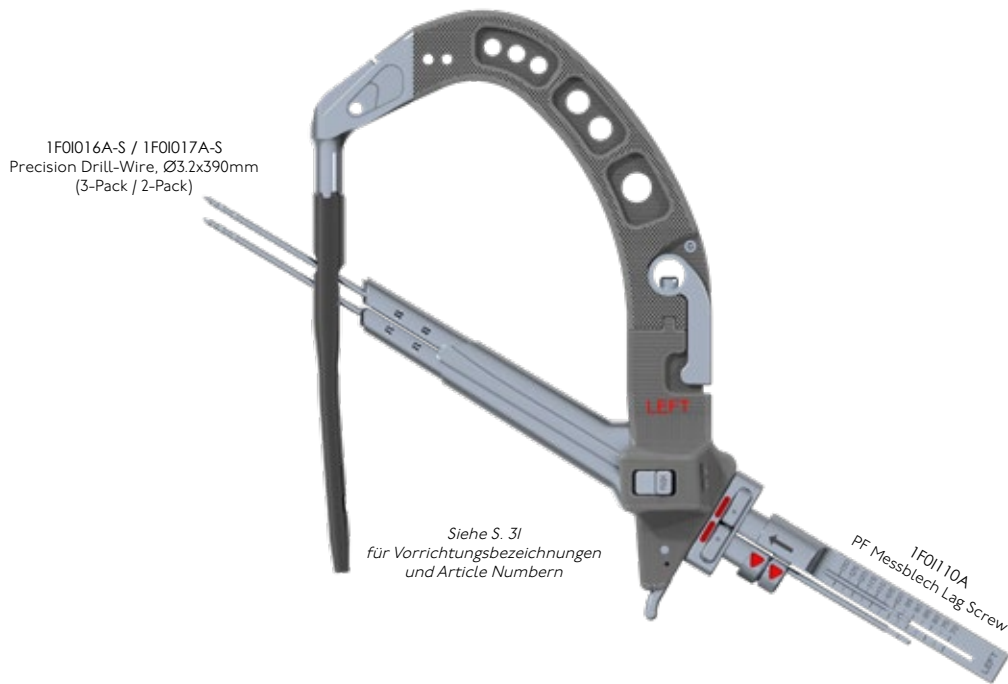


Lag Screw Drilling:

- The length for drilling and selecting the Lag Screw is determined using the Lag Screw Ruler (*PF Lag Screw Ruler*).

IMPORTANT: The measured value is 5mm shorter than the drill-wire and provides the length for the correct depth of drilling and selection of the Lag Screw.



- The depth stop (*Step Drill Depth Stop*) is placed onto the step drill (*PF Step Drill Lag Screw*) prior to the drill being attached to the power tool, and is then adjusted to the intended drilling depth, engaging in 5mm increments.

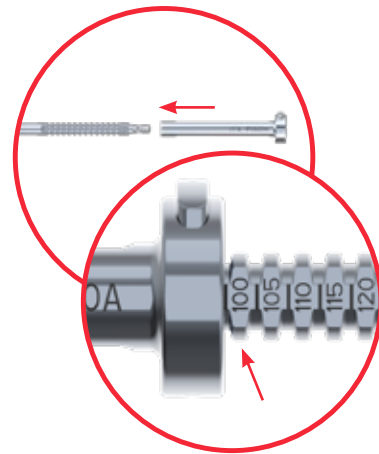

- The superior K-wire sleeve is removed for the drilling process, while the inferior K-wire sleeve continues to fix the correct alignment of the insertion guide and nail.

IMPORTANT: During the drilling, the inferior drill-wire remains inserted in the inferior K-wire sleeve, in accordance with the consistent doubling technique securing the head fragment against rotation.

- Insert the drill over the drill-wire, through the superior tissue protection sleeve and drill until the depth stop is reached.

IMPORTANT: The pre-set depth stop on the step drill prevents drilling too deep unintentionally. Nevertheless, it is recommended to check this process using the image intensifier, also to verify the final selection for the length of the Lag Screw.

IMPORTANT: If passage of the drill through the nail is obstructed, check to make sure that the drill-wire is not deflected.



- After drilling for the Lag Screw, the step drill is withdrawn.

IMPORTANT: After completion of the superior drilling process, the position of the superior drill-wire should be checked. If the drill-wire has moved during the drilling process, it should be repositioned.

TIP: If pre-tapping of the Lag Screw thread is necessary in case of very firm bone quality, a tap (*PF Lag Screw Tap*) is available, which can be mounted on the Lag Screw driver.

IMPORTANT: Since the tap has no calibration and no end stop, the cutting process should be performed under image intensifier control.



Lag Screw Insertion:



- The selected Lag Screw is placed on the Lag Screwdriver (*PF Lag Screw Driver*) and secured with the thread-carrying inner rod (*PF Lag Screw Driver Retaining Rod*).

IMPORTANT: The correct positioning is ensured by the asymmetrically designed connection. The grooves of the Lag Screw are correspondingly imitated on the shaft of the screwdriver for reliable position control.


IMPORTANT: Prior to the insertion of the Lag Screw, revalidate the attachment of the retaining screw (*PF Nail Holding Bolt*) to the nail to ensure it is secure.

- The cannulated Lag Screw is inserted into the soft tissue protection sleeve over the superior guide wire and screwed in maximally until to the end mark (black line on the lag screw driver) reaches the soft tissue protection sleeve.

TIP: This process is usually performed using the image intensifier.

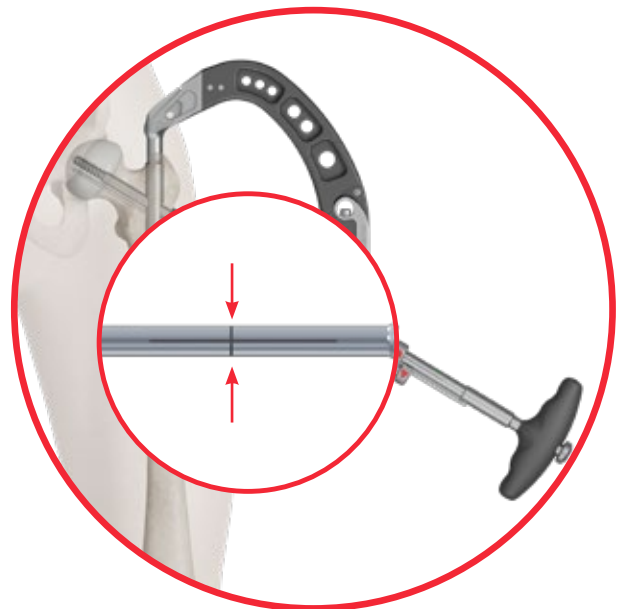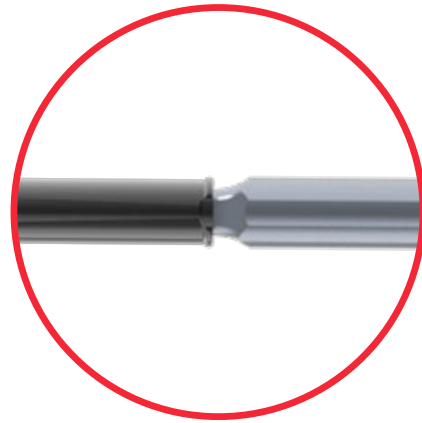

- The correct rotation position can be read off from corresponding markings on the soft tissue protection sleeve and the screwdriver shaft.
- Consequently, after a half turn and the corresponding 180° rotation of the Lag Screw, an end position can be found which simultaneously ensures correct insertion of the DyCon® Set Screw.

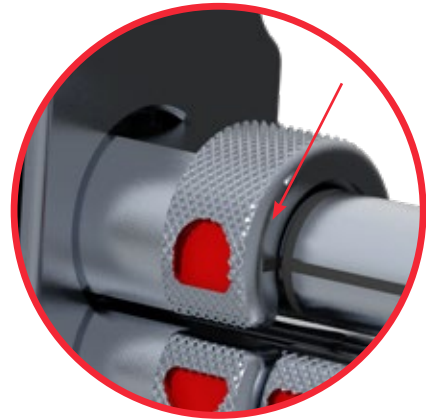

IMPORTANT: According to the pitch of the Lag Screw thread, this means a choice of final positioning in 1.6mm increments at a feed rate of 3.2mm per screw turn.


TIP: The rotational end position of the Lag Screw corresponds with a longitudinal orientation of the screwdriver handle in relation to the targeting device. This also references the orientation of the nail in the femoral shaft.

TIP: If reduction of a fracture gap by using the Lag Screw is desired, closing of the gap can be achieved using the apositioning instrument (*PF Apositioning Instrument*)- see p. 57.

- After final positioning of the Lag Screw, the lag screwdriver and Lag Screw drill-wire are removed.

Controlled Dynamization: DyCon® Set Screw Drilling & Insertion

Controlled Dynamization: DyCon®
Set Screw Drilling & Insertion

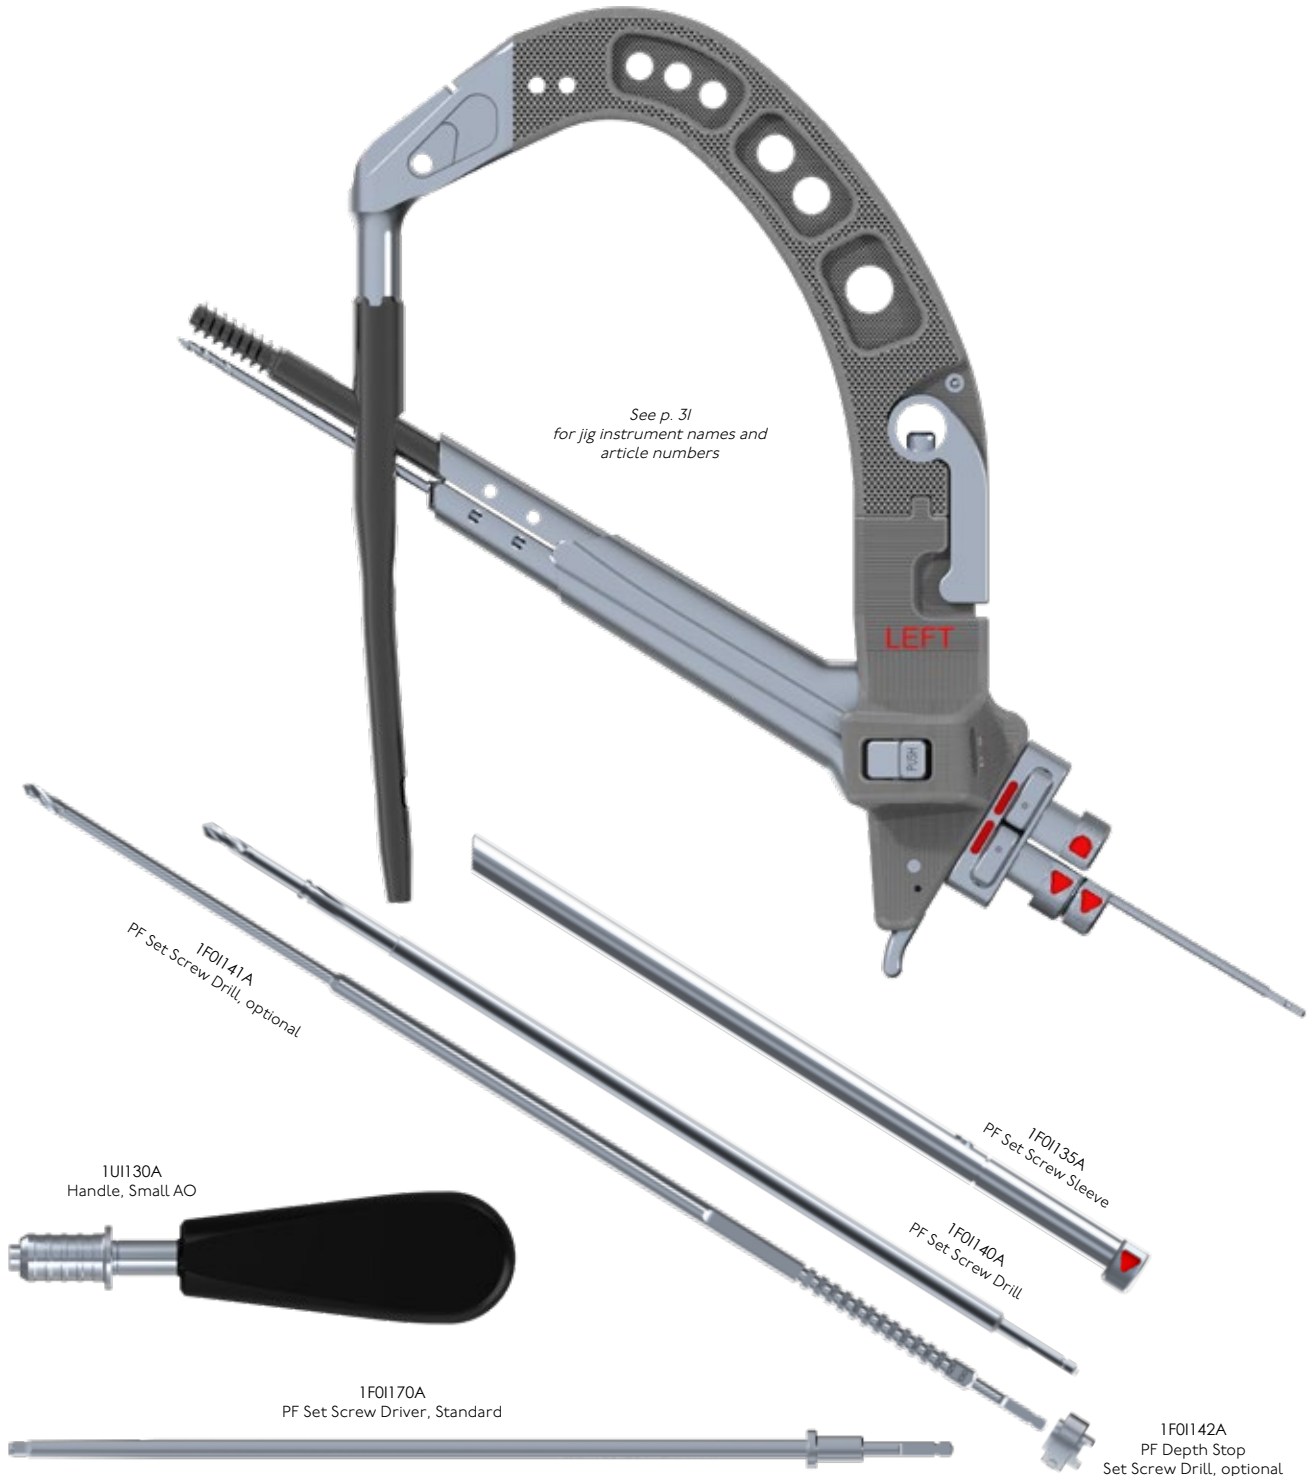

IMPORTANT: The standard technique describes the recommended dynamization of 5mm built in on the DyCon® Set Screwdriver (*PF Set Screw Driver, Standard with Handle, Small AO*).

IMPORTANT: Insertion and setting of the controlled dynamization do not differ for the long and short versions of the DyCon® Set Screw.

DyCon® Set Screw Drilling:


- The inferior drill-wire and inferior K-wire sleeve are removed and replaced by the Set Screw sleeve (*PF Set Screw Sleeve*).
- The length of the DyCon® Set Screw is selected corresponding to the Lag Screw inserted.

IMPORTANT: The long DyCon® Set Screw must be double-checked against the documentation or the packaging information for the inserted Lag Screw.

TIP: As an alternative to the rotation-locking standard DyCon® Set Screw, a short DyCon® Set Screw can also be selected (same design for all lengths of the Lag Screws).

- The Set Screw Drill (*PF Set Screw Drill*) is inserted through the set screw sleeve and used to drill until the stop is engaged.

TIP: Complete drilling can be checked using the image intensifier, upon which the indicator groove of the set screw drill should reach the lateral surface of the nail.

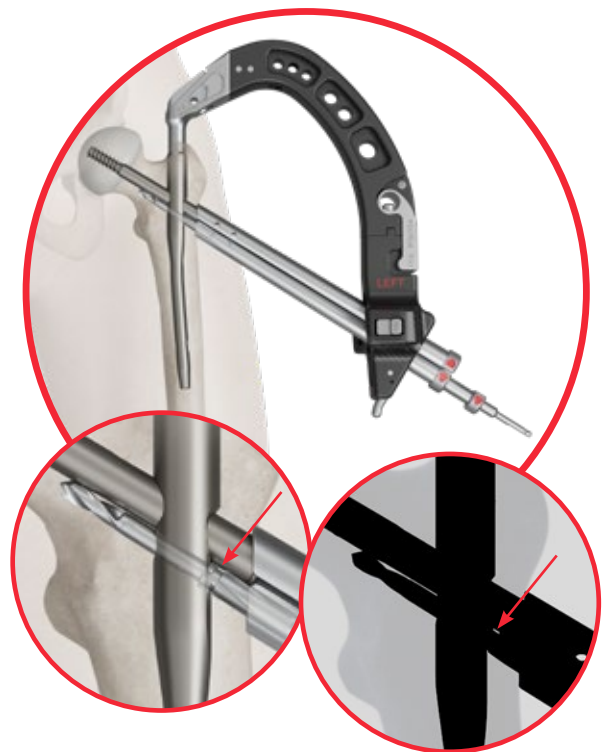

DyCon® Set Screw Insertion:

- The selected DyCon® Set Screw is picked up with the standard DyCon® Set Screwdriver (*PF Set Screw Driver, Standard with Handle, Small AO*) and inserted through the set screw sleeve, coming to rest in the groove provided by the Lag Screw.

TIP: The DyCon® Set Screw is first guided through the lateral femoral cortex with a slight twisting motion and then through the nail until the thread in the rear part of the DyCon® Set Screw engages with the corresponding thread in the nail.

IMPORTANT: When the DyCon® Set Screw reaches the predetermined depth, corresponding to 5mm dynamization, it is automatically pushed off the screwdriver.


TIP: If preferred, the dynamization distance can also be freely selected according to surgeon preference, see p. 58

TIP: If additional compression of the fracture is needed, see p. 60


TIP: In cases of good bone quality and/or a close proximation to the Adam's arch the path of the set screw can be cleared out by a drill (*PF Set Screw Drill, optional*) with a corresponding depth stop (*PF Depth Stop Set Screw Drill, optional*).

Furthermore a possible distraction of the head/neck fragment can be avoided.

The drill depth must be chosen in accordance to the lag screw length.

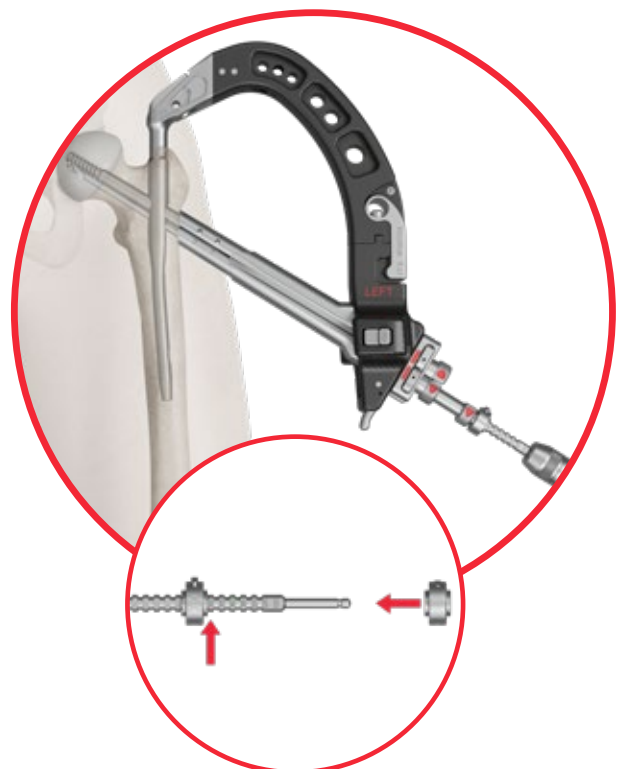

○ Guided Distal Locking

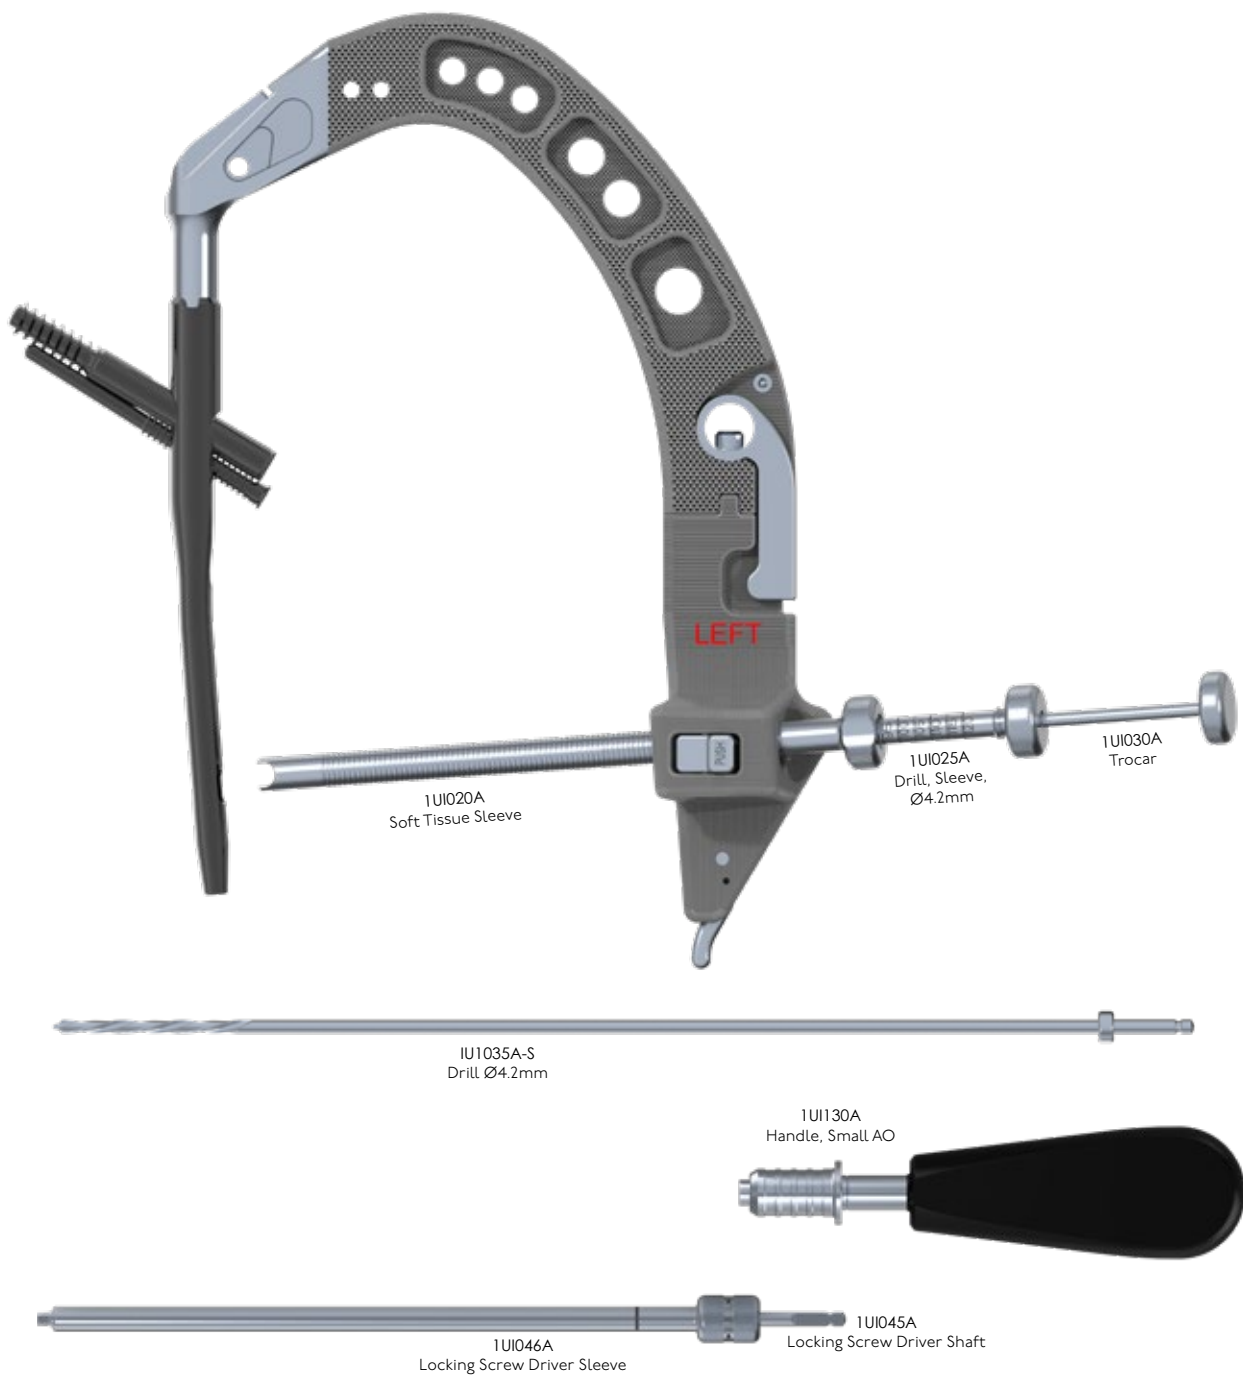


Distal locking is performed identically for the short (*PF Nail, short*) and intermediate (*PF Nail, intermediate*) nail via the holes located on the Targeting Module PF with the alternatives of an superior/cranial and thus static or inferior/caudal and thus dynamic screw position.

The freehand distal locking procedure for the long nails is described separately - see p. 68


- The sleeve package for the distal 5mm locking screw is assembled (*Soft Tissue Sleeve, Drill Sleeve, Ø4.2mm and Trocar*).
- A separate stab incision is performed of the skin and fascia down to the bone.
- The sleeve package is then inserted through the selected static or dynamic position in the targeting module, and advanced through the soft tissue incision to the bone. The position is secured using an automatic ratchet mechanism.

IMPORTANT: To ensure correct measurement, make sure the sleeve package is seated close against the lateral cortex, causing the trocar to "pop off" the end of the drill sleeve.

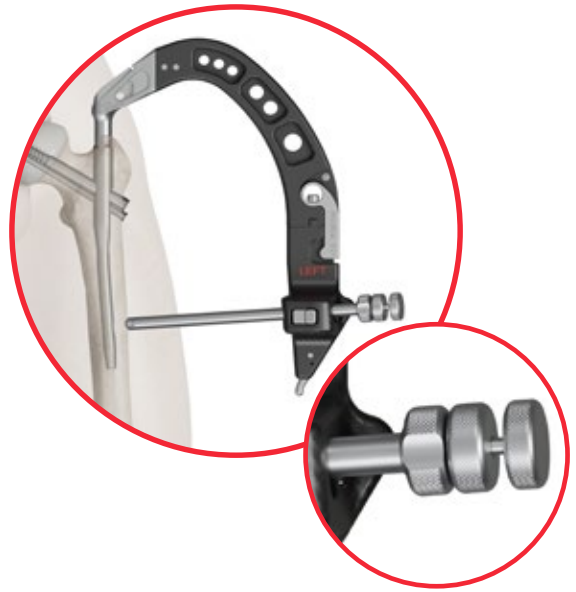

- After removing the trocar, the calibrated drill (*Drill, Ø4.2mm*) for the 5mm locking screws (*Locking Screw Ø5mm*) is first predrilled through the lateral cortex of the nail and the medullary canal to the easily felt medial inner cortex.
- In this position, the drill sleeve is unlocked from the soft tissue protection sleeve and pulled back to the stop on the 4.2mm drill bit.
- The length of the screw up to the inner medial cortex can be read on the drill sleeve and then the necessary screw length calculated with an addition for the medial cortex.

IMPORTANT: For osteoporotic bone, an addition of 5mm may be sufficient. If the cortex is strong, a 7.5 or 10mm longer screw should be selected.

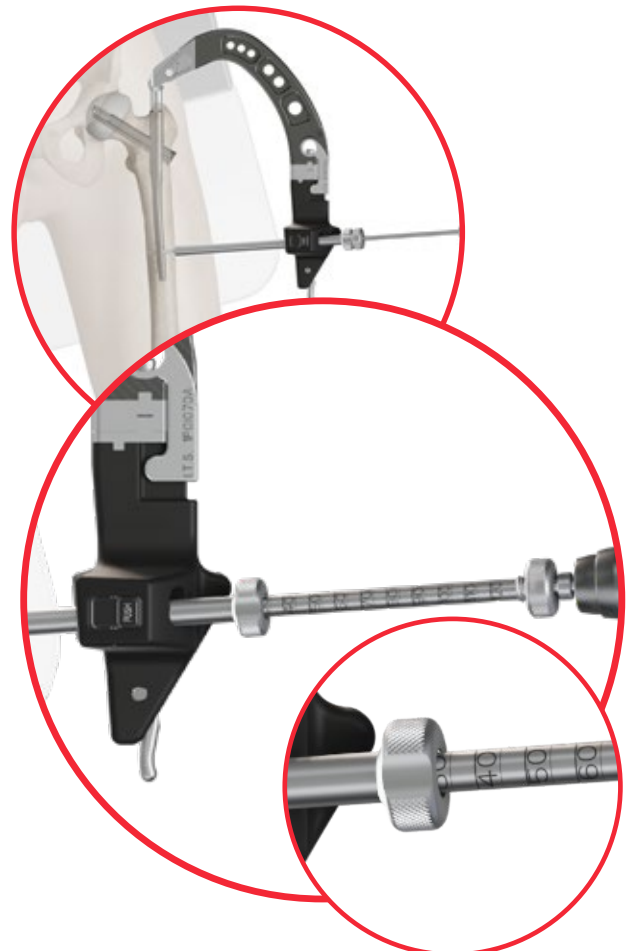


- Next, the medial cortex is overdrilled.


ALTERNATIVE: The screw gauge (Screw Gauge) can be used through the soft tissue sleeve after the drilling of both the lateral and medial cortices has been completed.

- The drill with the drill sleeve is then removed.
- The screwdriver shaft and sleeve are assembled (Locking Screw Driver Shaft and *Locking Screw Driver Sleeve*).
- The selected self-tapping locking screw is then picked using the Locking Screwdriver and screwed in.

TIP: In the case of strong cortical bone with a high insertion resistance, this process can be performed with the image intensifier, whereby the approach of the screw head in the final position to the lateral cortex can be easily observed via a recess in the soft tissue sleeve and a mark on the screwdriver.

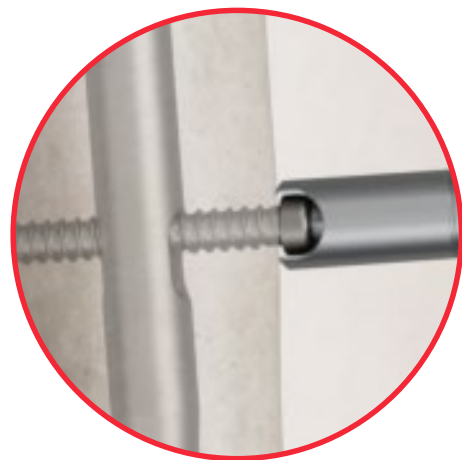

- Once the screw reaches the final position, the screwdriver is released by turning the screwdriver sleeve in the “RELEASE” direction marked on the sleeve.



○ Disassembly of Targeting Arm

- Once the DyCon® screw pair has been placed as well as the distal locking screw, the Targeting arm can be disassembled from the nail by removing any remaining sleeves and then unscrewing the nail retaining bolt.
- The final step is to decide whether an end cap should be placed in the nail after removal of the insertion guide. For the placement of an optional end cap / axial set screw - see p. 62.

○ Rotation Control and Image Intensifier Documentation

- The rotation of the leg is 12° when the aiming sleeve for the distal locking is in line with the plane of the femoral condyles and the Lag Screw is in the center of the femoral head.

TIP: The position of the femoral condyles can be verified with the image intensifier and is ideally parallel to the floor at the beginning of surgery. The final clinical visual check can then be limited to establishing the parallel position of the drill sleeve inserted in the insertion handle (as an indicator for distal locking) in relation to the floor.

IMPORTANT: Before performing the final image intensifier check, all soft tissue protection sleeves, the master sleeve and the modular insertion handle portion are first removed.


- The hip joint and the proximal femur with the full nail are adjusted in the a/p projections.
- The image intensifier is then rotated into the lateral projection of the femoral neck and the positions of the Lag Screw in the femoral head and the distal locking screw are checked.

IMPORTANT: The reduction, implant position and screw lengths are verified, with final documentation via paper printouts or integration into the hospital electronic documentation system.

○ Wound Closure & Follow-up

- Wound closure is performed in the conventional manner in layers at the surgeon's discretion with or without suction drains.
- The postoperative weight-bearing capacity should be adapted to the fracture situation, where, especially for elderly patients, a full load bearing with walking aids is to be aimed for.
- With sufficient intraoperative image intensifier controls with corresponding documentation, standardized X-ray images in two planes should be performed before inpatient discharge, as well as at follow-up after 4-6 weeks and with documentation of fracture healing after 3-6 months.

○ OPTIONAL: Correction of Trochanteric Entry Point

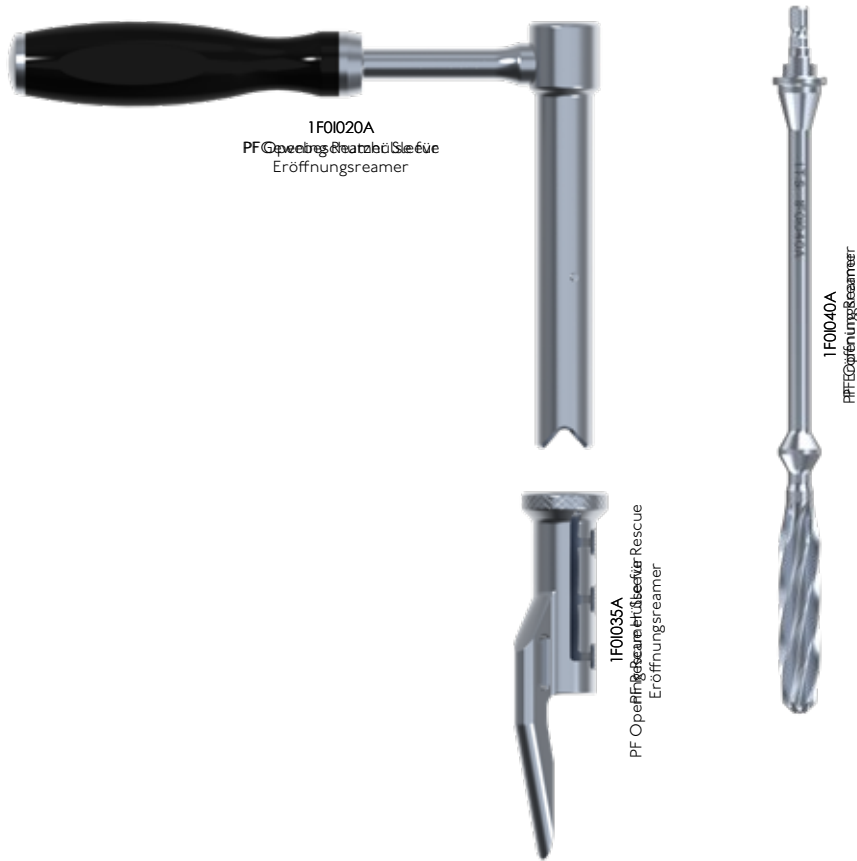


If there is a deviation of the drilled trochanteric entry point, the hole can be repositioned using the rescue sleeve (*PF Opening Reamer Sleeve Rescue*).


The rescue sleeve allows for the opening to be adjusted either laterally or medially to three separate distances.

- The opening drill-wire, the multihole trocar and the opening reamer sleeve are removed.
- The rescue sleeve is assembled onto the opening reamer sleeve and one of the three possible adjustment distances (5mm, 10mm, 15mm) is selected.

- The opening reamer sleeve is reintroduced to the intramedullary canal such that the rescue sleeve protrudes into the medial side for a lateralization of the entry point and the lateral side for a medialization.
- The medullary canal opening is then re-drilled through the opening reamer sleeve using the opening reamer.

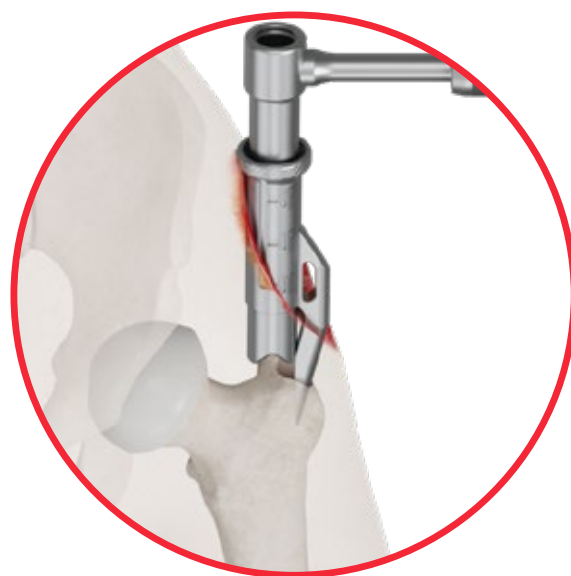

○ OPTIONAL: Correction of Lag Screw Drill-Wire

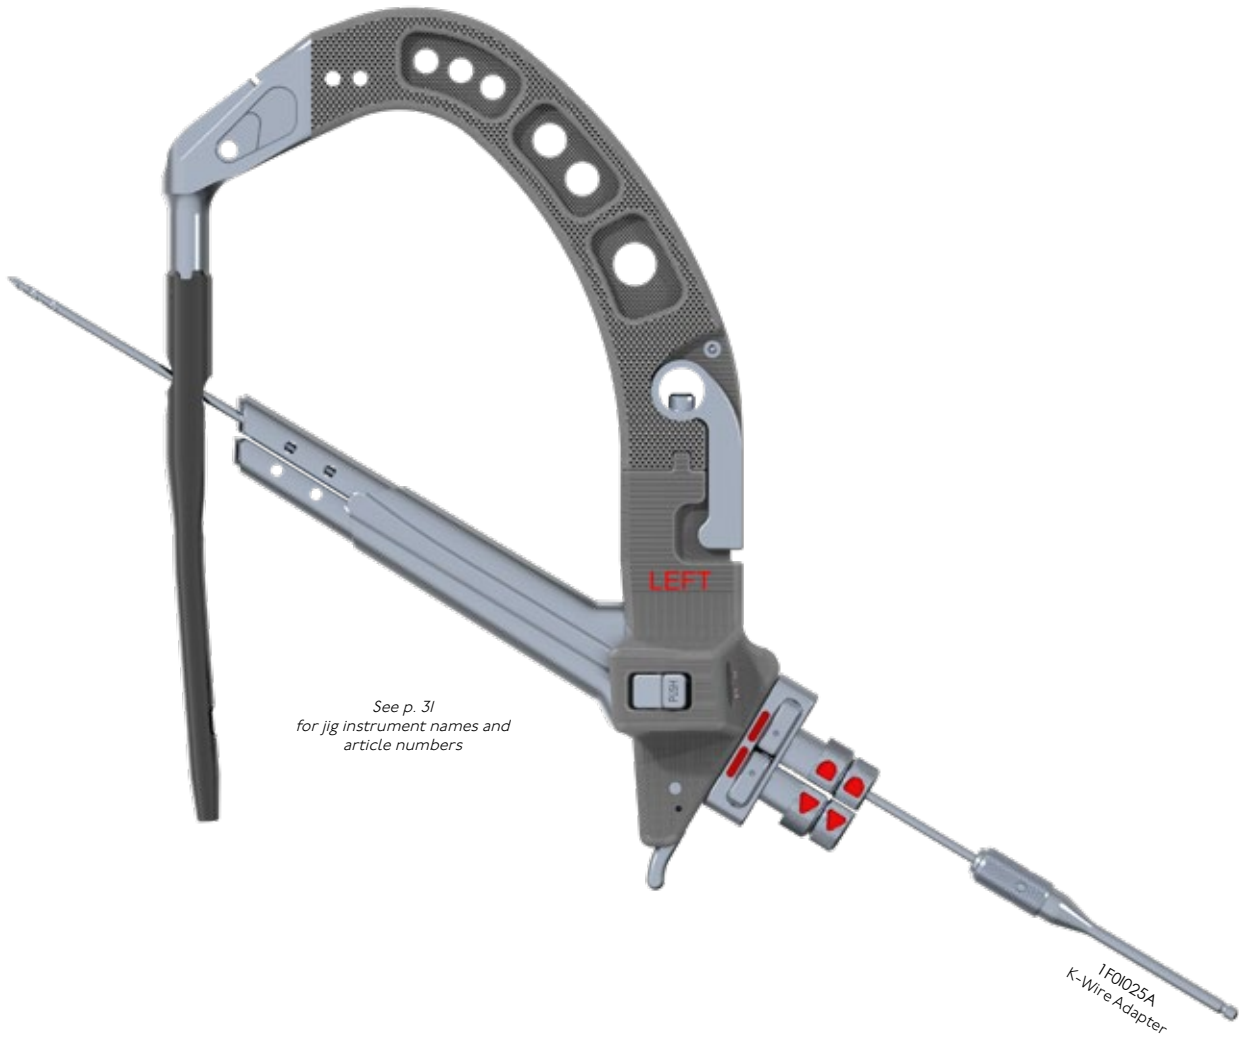

If a deviation of the superior drill-wire cranially or caudally is detected during the a/p image intensifier check, it is, thanks to the parallel trajectories of the two drill-wires, possible to adjust the drill-wire positioning, while retaining the correct central position in the lateral projection.

With the application of these described positioning steps, the superior drill-wire, which is decisive for the subsequent position of the Lag Screw, can be corrected by 8.5mm both caudally and cranially.

Correction to a superior position:

- Both K-wire sleeves are removed.
- The nail, jig and master sleeve with tissue protection sleeves are shifted cranially until the drill-wire is in line with the alignment holes in the inferior tissue protection sleeve.

IMPORTANT: The drill-wire is checked in the image intensifier to ensure that it has reached the center of the DyCon® Set Screw hole in the nail.

- The inferior K-wire sleeve is inserted over the drill-wire (now in the inferior position).
- The superior K-wire sleeve is inserted into the superior tissue protection sleeve and the new superior drill-wire is placed through the superior K-wire sleeve.




Correction to an inferior position:


- A second drill-wire is placed through the inferior K-wire sleeve, becoming the central drill-wire for the Lag Screw.
- The superior drill-wire and both K-wire sleeves are removed.
- The nail, jig and master sleeve with tissue protection sleeves are shifted caudally until the remaining drill-wire is in line with the alignment holes in the superior tissue protection sleeve.

IMPORTANT: The drill-wire is checked with the image intensifier to ensure that it has reached the center of the Lag Screw hole in the nail.

- The superior K-wire sleeve is inserted over the corrected drill-wire (now in the superior position).
- The inferior K-wire sleeve is then inserted into the inferior tissue protection sleeve and the inferior drill-wire is placed through the inferior K-wire sleeve.

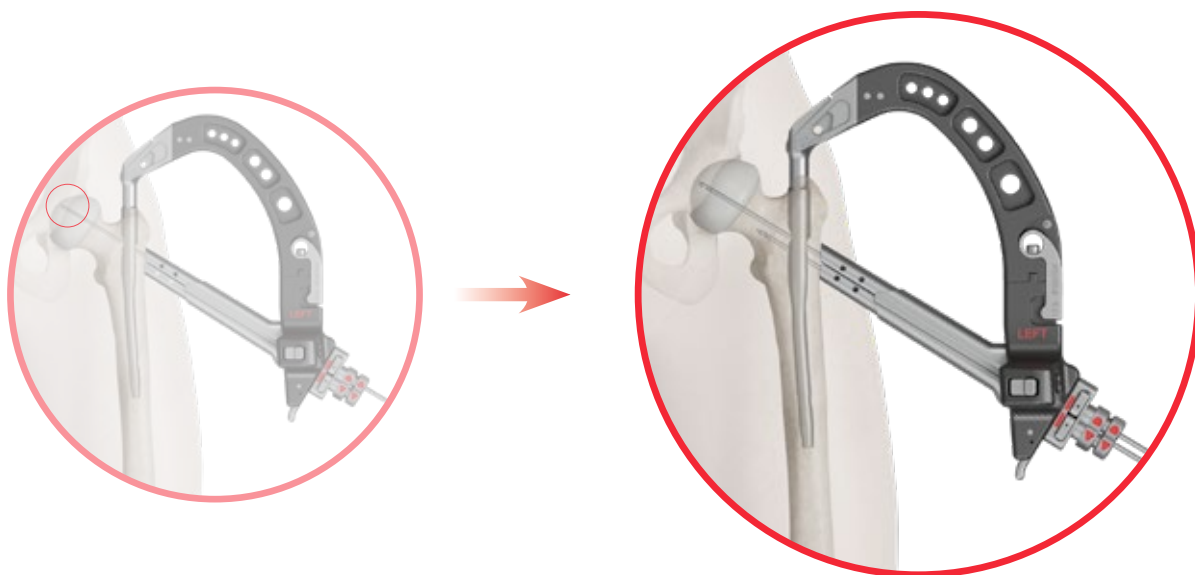

○ OPTIONAL: Closure of a Fracture Gap

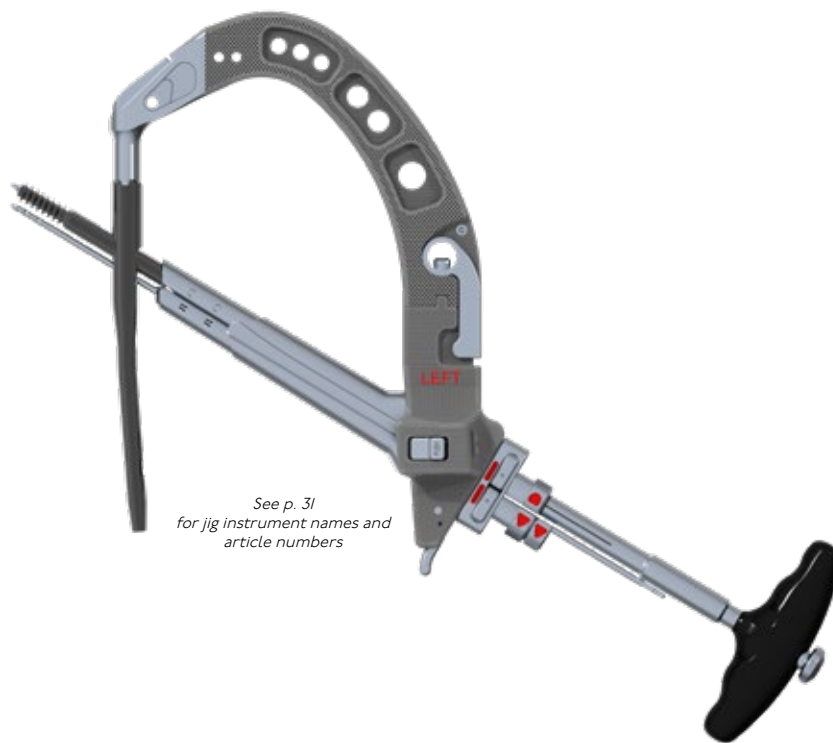

If closing of a fracture after insertion of the Lag Screw is desired, force can be applied between the tissue protection sleeve and the screwdriver by means of the apositioning instrument (PF Apositioning Instrument).


- The apositioning instrument is positioned onto the shaft of the screwdriver such that the ends are in contact with the end of the superior tissue protection sleeve and the screwdriver.

TIP: The pin in the middle position represents the calibrated final position of the Lag Screw. If the Lag Screw is screwed in more or less than the indicated line, the apositioning instrument can be adjusted by moving the pin* to one of the external holes.

- Pressure is applied to the handle of the apositioning instrument, forcing the ends apart and thus closing the fracture gap.

IMPORTANT: This step is usually performed with caution under image intensifier control.

TIP: If sufficient closure cannot be reached, the traction settings should be reduced.

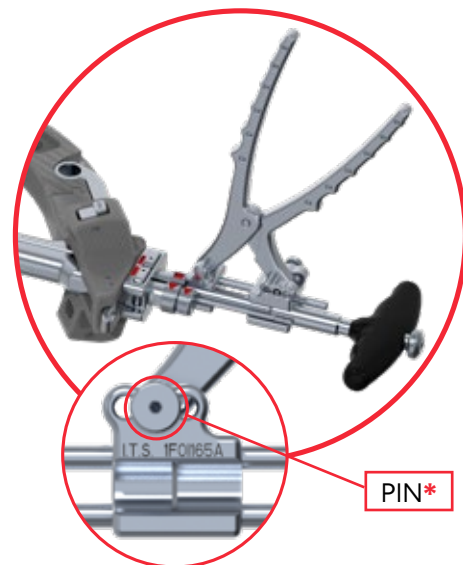




DyCon® Set Screw Insertion:

- For freely selectable dynamization, the selected DyCon® Set Screw is picked up with the optional DyCon® Set screwdriver (*PF Set Screw Driver, Optional with Handle, Small AO*) and inserted through the set screw sleeve, to the desired depth in the groove provided by the Lag Screw.


TIP: The DyCon® Set Screw is first guided through the lateral femoral cortex with a slight twisting motion and then through the nail until the thread in the rear part of the DyCon® Set Screw engages in the corresponding thread in the nail.

IMPORTANT: The depth to which the DyCon® Set Screw is screwed in determines the potential lateral dynamization distance for the Lag Screw. This is indicated by the laser markings on the screwdriver referenced against the set screw sleeve.

IMPORTANT: If inserted further than the markings the fracture may be distracted.

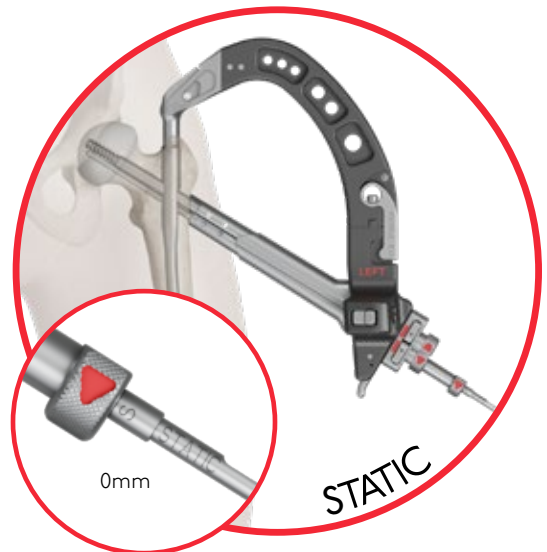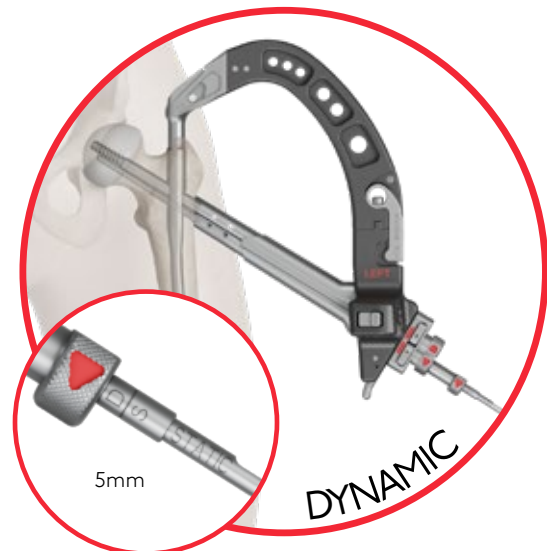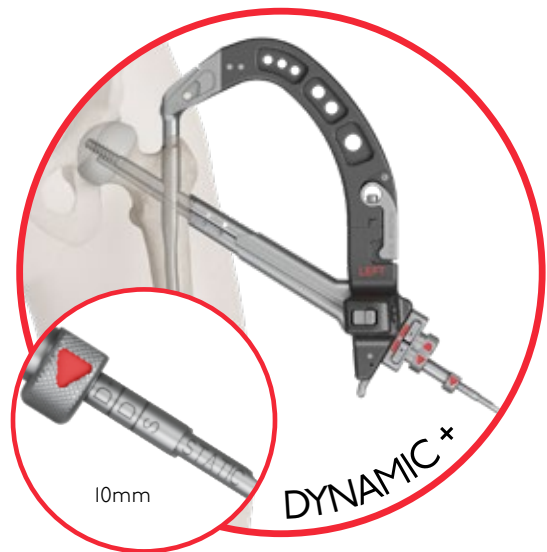

○ OPTIONAL: Advanced Compression

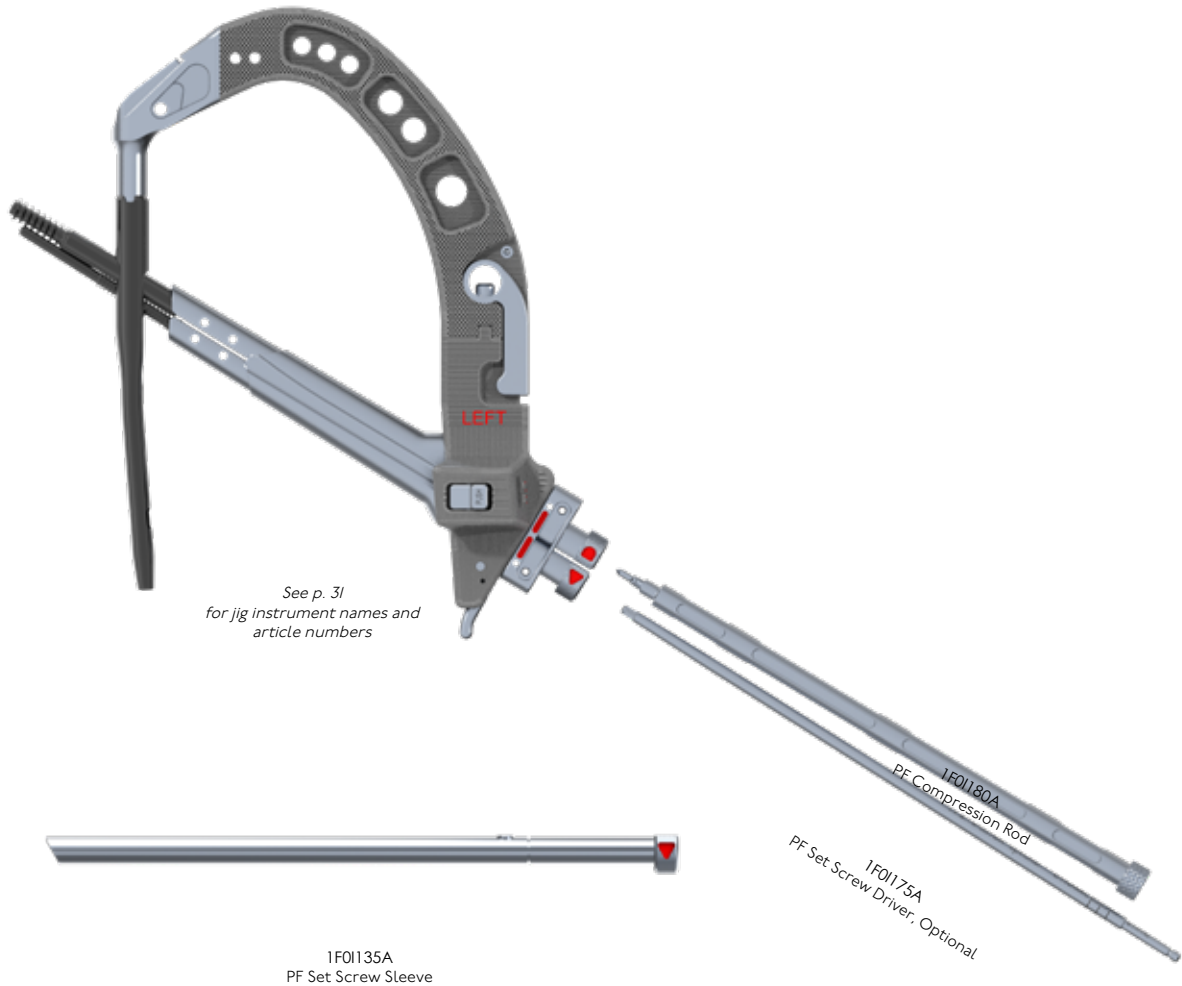

The Compression Rod (PF Compression Rod) allows the DyCon® Screw pair to be pulled laterally by a slight unscrewing of the DyCon® Set Screw.

IMPORTANT: The Advanced Compression technique requires a selected dynamization mode of 5mm or less (Dynamic or Static modes). If a greater dynamization has been dialed in (Dynamic+), the DyCon® Set Screw must first be screwed further in to Dynamic Mode (indicated by the laser markings on the screwdriver opposite the set screw sleeve) in order to allow the Compression Rod to engage with the Lag Screw.

IMPORTANT: If the set screw sleeve was used to check the dynamic mode. It must be removed again.


- The compression rod is screwed into the Lag Screw.
- The optional DyCon® Set Screwdriver (*PF Set Screw Driver, Optional with Handle, Small AO*) is inserted into the set screw and turned anticlockwise to create compression.

IMPORTANT: Compression should be performed with caution under image intensifier control.

- When the desired compression is achieved, the screwdriver and compression rod can be removed. The standard dynamisation of 5mm (Dynamic mode) is set.
- If a different locking mode is desired, the set screw sleeve is used in conjunction with the screwdriver. The orientation follows the laser marking - see p. 59.



OPTIONAL: End Cap Screws & Axial Set Screw

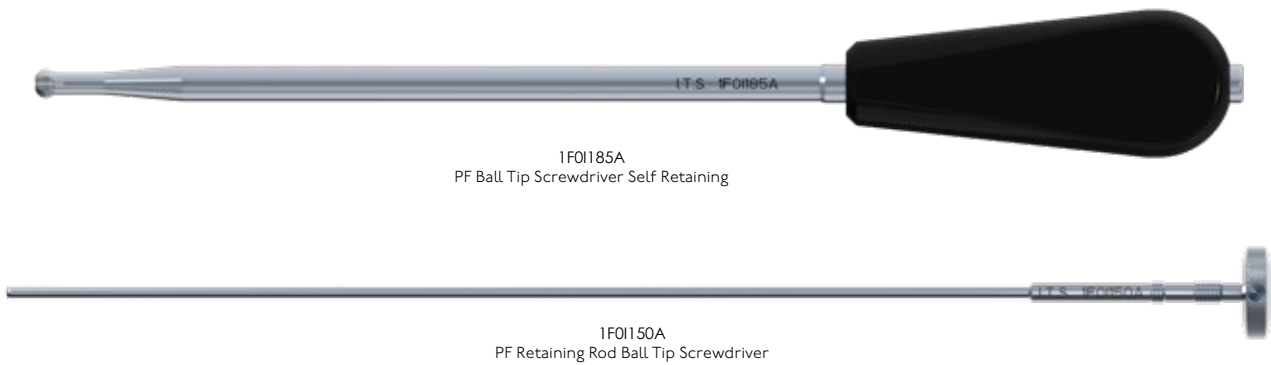

IMPORTANT: In the majority of clinical situations, this surgical step is dispensable and can be saved in terms of time and material. Indications for end caps exist if, for example, the thread is to be kept free of scar tissue for a planned implant removal, if an extension of the proximal nail end is desired, or for rotational locking of the Lag Screw in the absence of a DyCon® Set Screw.

- The end cap screws are available with a proximal extension of 0 to 20mm in 5mm increments.
- Secure the selected endcap to the Ball-tip Screwdriver (*PF Ball tip Screwdriver Self Retaining*) using the corresponding retaining rod (*PF Retaining Rod Ball Tip Screwdriver*).
- Screw the endcap in until a contact is felt to the groove of the Lag Screw.

IMPORTANT: It is not necessary to turn the end cap screw back after tightening. When screwed in the upper groove of the Lag Screw, all end cap screws block rotation. However, the design principle allows the Lag Screw to continue to slide dynamically in a lateral direction.

○ LONG NAILS:
Reduction of the Shaft Fracture &
Reaming of the Medullary Canal

1UI125A
T-Handle Zimmer Hall, Cannulated



1UI120A
Reduction Rod



1UI095A-S
Ball Tip Guide Wire, Ø3x800mm



1UI100A
Guide Wire Pusher



1UI224A
Fixed Head Reamer, Ø10mm




1UI200A
Modular Reamer Shaft, Ø8x475mm




1UI258A / 1UI260A / 1UI262A / 1UI264A / 1UI266A 1UI268A
Modular Reamer Head, Ø11mm / Ø12mm / Ø13mm / Ø14mm / Ø15mm / Ø16mm



1UI090A
Gripper

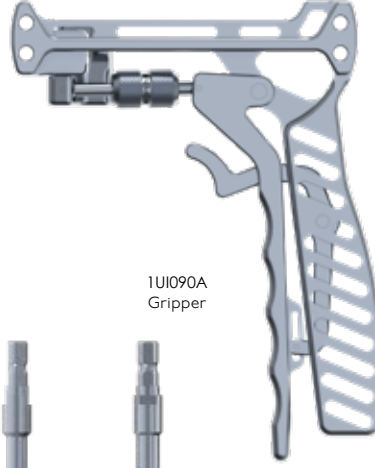

1UI010A
PF X-Ray Ruler, Long



LONG NAIL:
Reduction & Reaming

- The ball tip guide wire (*Ball Tip Guide Wire, Ø3x800mm*), which can be slightly bent at the end area. It is then inserted into the medullary canal using the wire holder (*Gripper*).
- The wire is inserted into the distal fragment under the control of the image intensifier.

TIP: A reduction instrument (*Reduction Rod*) can be inserted over the guide wire into the medullary canal, thus enabling manipulation to bring the proximal fragment into a suitable position.

ALTERNATIVE: If the fractures are displaced and cannot be reduced on the fracture table, for example subtrochanteric fractures, a lateral position on a radiolucent table without traction can be used. In these cases, the reduction is carried out using an open technique with temporary fixation using reduction forceps. An additional fixation using wire cerclage has also proven successful. Nailing can then be carried out safely in the reduced and anatomically fixed position. In the case of shaft fractures, it is also possible to treat the patient in the lateral position.

- The medullary reaming wire is anchored precisely in the center of the cancellous bone in the distal femoral metaphysis.

IMPORTANT: The distal central placement of the medullary reaming wire is essential for the quality of the reduction by the nail itself with the alignment of the long axis of the femur.

- In this final position, the length measurement is checked by evaluating the protruding end of the ball tip guide wire with the guide wire ruler (*Guide Wire Ruler, Long*) as a subtraction measurement with direct length reading.



- Beginning with the front-cutting medullary reamer, reaming is carried out in 1mm and, if necessary, 0.5mm increments.

TIP: *3-step reaming guide*

Proximal: Opening Reamer


Isthmus: 2mm more than selected nail

Distal: Same diameter as selected nail

IMPORTANT: If the medullary reamer comes into direct contact with the hard cortex in the isthmus, a 2mm larger reamer is then used to ensure safe passage of the intramedullary nail.

TIP: To ensure that the ball-tip guide wire remains in the correct position when the intramedullary reamer shafts are withdrawn, it should be held in position with the guide wire pusher (*Guide Wire Pusher*).

LONG NAILS: Insertion of the Long Intramedullary Nail

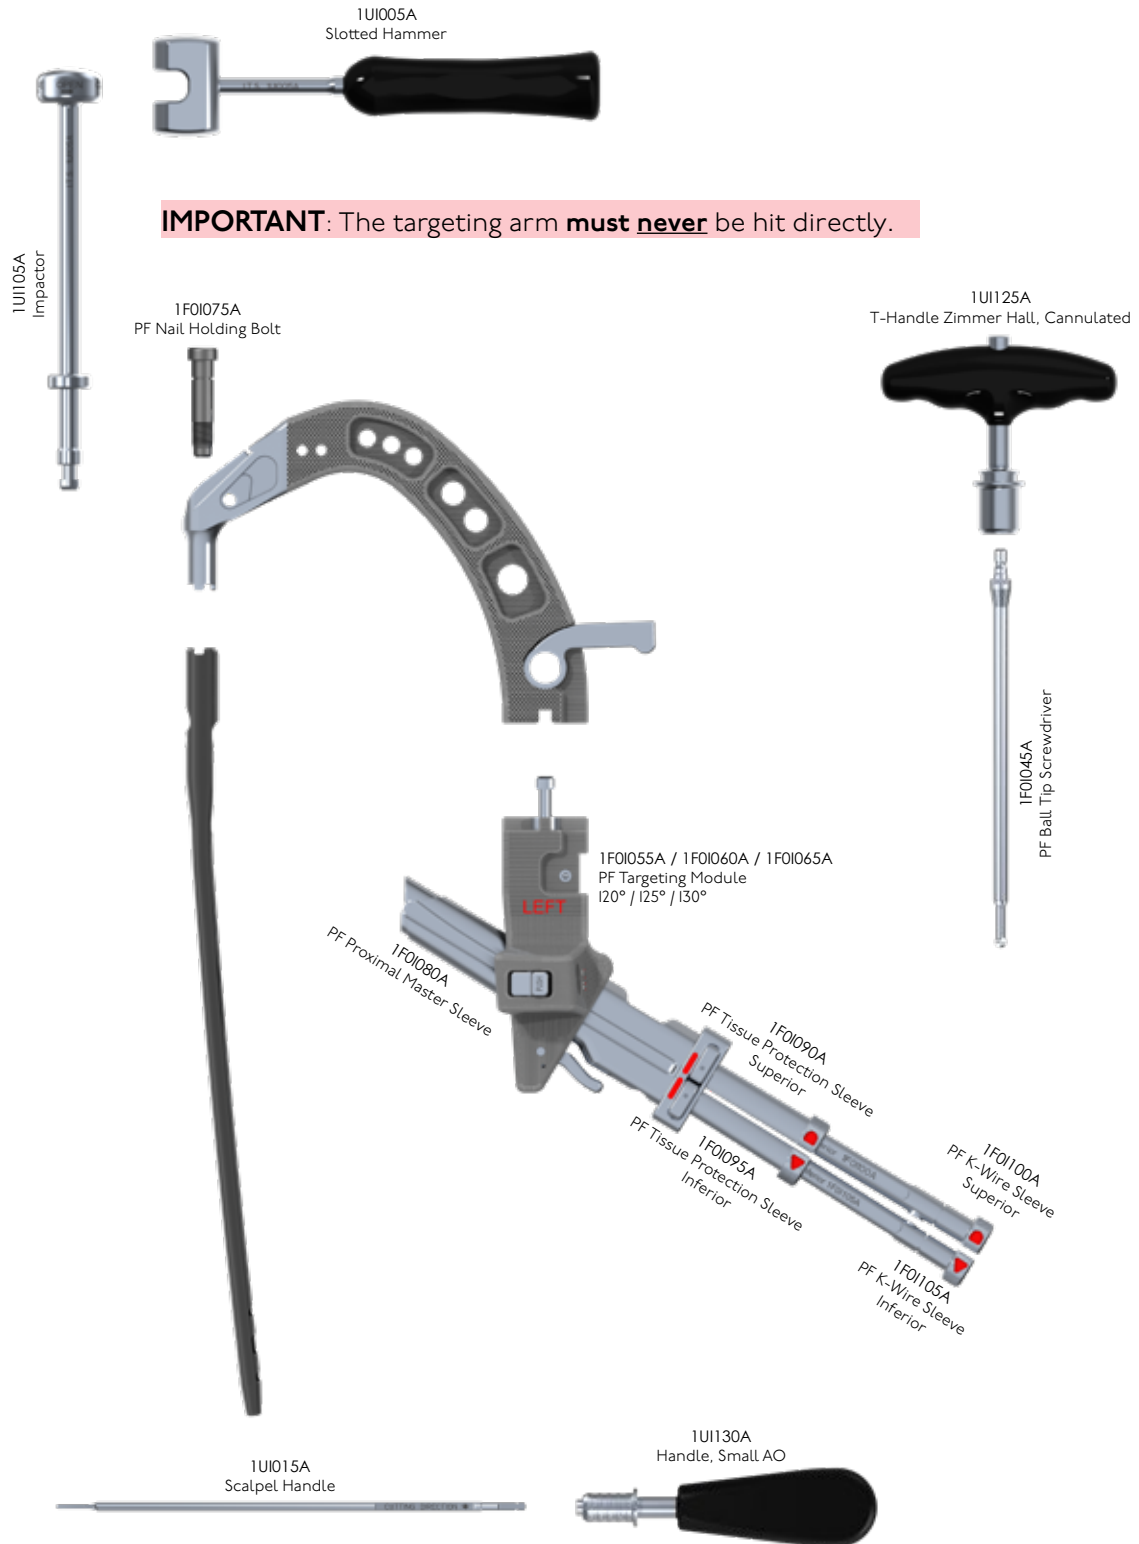

IMPORTANT: The targeting arm **must never** be hit directly.

LONG NAILS: Nail Insertion

- The long medullary nail is selected with regard to length, femoral neck angle and diameter.
- The nail is attached to the targeting arm by a ball-tip screwdriver (*Targeting Arm with Locking Lever, PF Nail Holding Bolt, PF Ball Tip Screwdriver incl. T-Handle Zimmer Hall Cannulated*).


IMPORTANT: The targeting module (*PF Targeting Module 120°, 125° or 130°*) must be double-checked for compatibility with the femoral neck angle of the mounted nail.

IMPORTANT: The retaining screw (*PF Nail Holding Bolt*) securing the nail must be fully tightened to ensure that the nail does not loosen during insertion.

- The long intramedullary nail is inserted proximally over the ball-tip guide wire in such a way that the aiming arm is first turned anteriorly in order to use the antecurvature of the implant for passage through the entry route.
- When the isthmus is reached latest, the nail is turned back into the normal position, corresponding to a nearly horizontal position of the targeting arm.

TIP: For the final positioning of the nail, the impactor can be used for the fine-adjustments, both to impact and retract. For this, the impactor must be mounted on the aiming arm.

IMPORTANT: The targeting arm **must never** be hit directly.

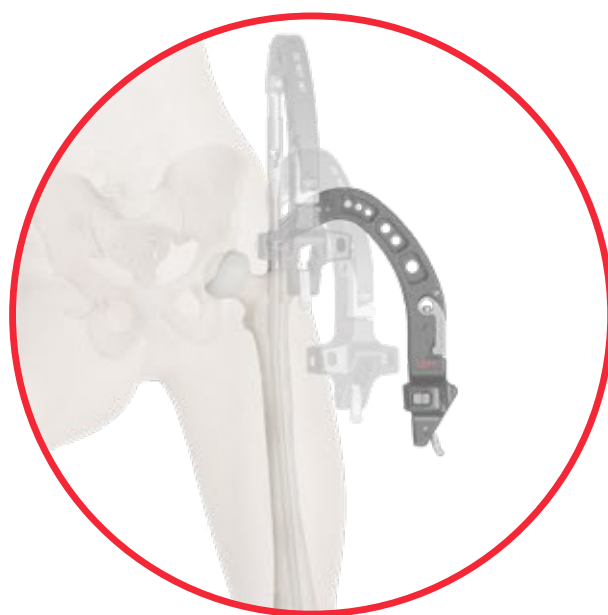

The next steps in the procedure for using the long intramedullary nails follows that of the standard technique from the section on the insertion of the Master Sleeve and checking implantation depth and onwards - see p. 31.

LONG NAILS: Free-hand Distal Locking

1UI069A-S
Bohrer Freihandverriegelung, Ø4.2x120mm, STE



1UI070A-S
Bohrer Freihandverriegelung, Ø4.2x170mm, STE




1UI071A-S
Bohrer Freihandverriegelung, Ø4.2x220mm, STE



1UI065A
Measuring Sleeve



1UI060A
Screw Gauge



1UI055A
Capture Sleeve



1UI050A
Locking Screw Driver, Short



1UI130A
Handle, Small AO



The distal locking when using the long nails can be carried out using one of the numerous freehand techniques, as chosen by the surgeon. The technique described here enables rotation control of the femoral axis using the image intensifier in the lateral projection of the distal femur.

A correct central position of the DyCon® Lag Screw with 12° anteversion of the femoral neck opens the possibility of rotation control via the distal freehand locking.

- After the final placement of the DyCon® screw pair, the image intensifier is set in an exact lateral projection above the knee joint.

TIP: Assuming normal anatomy, the exact lateral projection is achieved when the medial and lateral femoral condyles project onto one another identically.

- In this image intensifier position, the distal end of the nail is moved into view and checked to determine whether the two round holes are projecting exactly circular. If this is not the case, the proximal femur part should be rotated using the aiming device until a circular projection results.


IMPORTANT: This position ensures that there is an anteversion of the femoral neck of 12° with a neutral femoral axis.

- Stab incisions are then placed over those holes that have been selected for locking.

TIP: Depending on the clinical situation, the two round holes are usually filled, which leads to a static locking. If a dynamic locking situation is desired, the elongated hole is filled in the lower position. This position is also selected if later dynamization is to be made possible by removing the two static screws.



- The drill (*Drill Freehand, Ø4.2 x 120mm*) is positioned under image intensifier control, through the stab incision in a slightly inclined position with its tip exactly above the center of the base hole.
- The tip of the drill is anchored in the cortex by gently engaging the drill.
- The power tool with the drill is then swiveled into the exact central position seen in the image intensifier.
- The first lateral cortex is drilled, and making sure the nail is passed, the second, medial cortex is drilled.
- The length is measured by a measuring gauge (*Screw Gauge*) with a measuring sleeve (*Measuring Sleeve*).
- The selected screw is then screwed in using the Locking Screwdriver for freehand locking (*Locking Screw Driver, Short*).

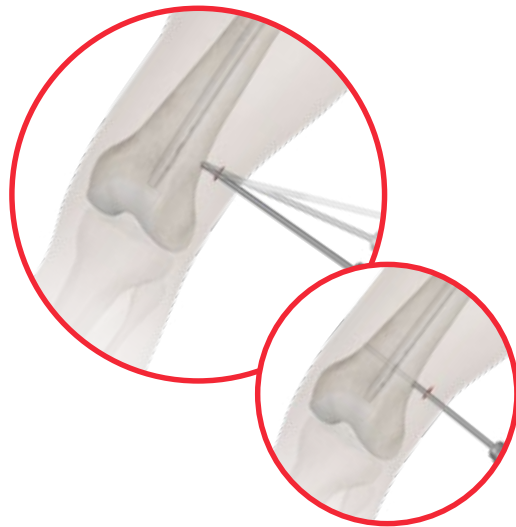


TIP: For screw insertion, the screwdriver can be used with an optionally available locking sleeve (*Capture Sleeve*).

- After inserting the screws, the position is documented with the image intensifier in two planes.

TIP: Ideally both the screws and the femoral condyles should be shown exactly laterally in the lateral projection.

The completion of the operation when using the long nails now corresponds to the procedure for the standard technique - see p. 50.

○ Implant Removal

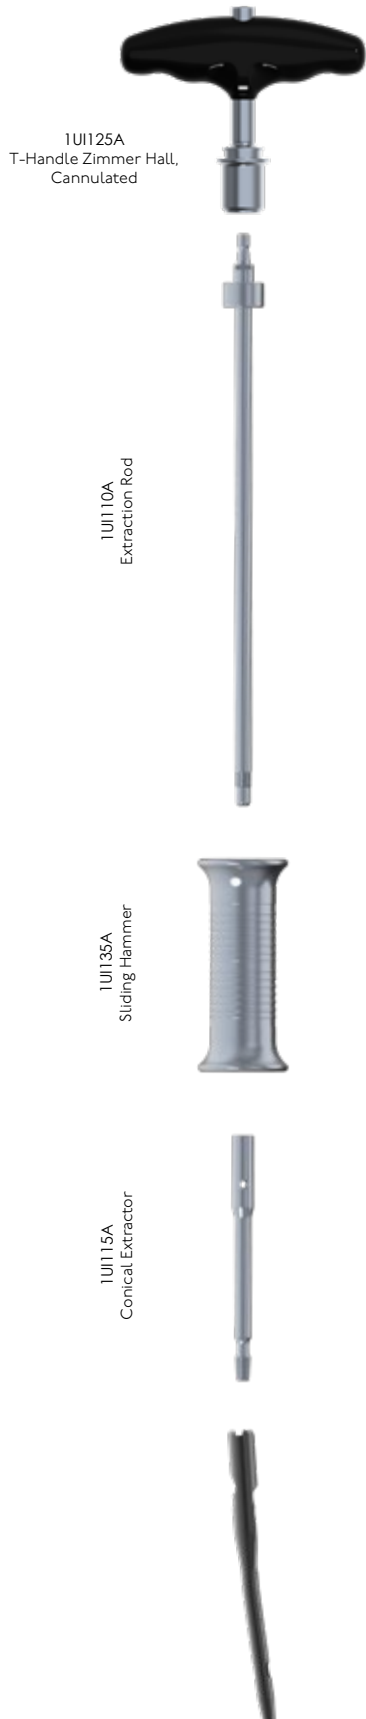

Removal of implants usually is indicated only in younger patients. Exceptions are local irritation, for example in a thin patient with a limited soft tissue envelope and lateral migration of the femoral neck screw.

To perform the implant removal, the identical instruments should be available as for insertion of the nail, with the exception of the targeting instruments and sleeves.

NOTE: After implant removal, especially in the case of osteoporosis, increased incidence of femoral neck fractures has been described in literature.

- After excision of the scars, the original surgical approaches are used and the nail head, the DyCon® Screw Pair and the distal locking screws are exposed.

NOTE: The Lag Screw can only be unscrewed after complete removal of the DyCon® Set Screw and End Caps.

IMPORTANT: The distal locking screw should not be unscrewed until the explantation instruments are securely connected to the nail head.

- First, the conical nail connection (*Conical Extractor*) is mounted to the extraction rod (*Extraction Rod*) by means of a screw connection. If the sliding hammer (*Sliding Hammer*) is to be used, it is first placed onto the extraction rod.
- Attach the T-handle and screw this construct into the nail connection. (If an end-cap is in place, it has to be removed prior.)
- Alternatively, the construct can be removed using the slotted hammer.

NOTE: Before striking the nail, it must always be ensured once again that all screws originally crossing the nail have been safely removed, especially the distal locking screws.



Information

3.

○ Typ II Anodization


Chemical process - anodization in a strong alkaline solution*

Type III anodization

- Layer thickness 60-200nm
- + Different colors
- Implant surface remains sensitive to:
 - Chipping
 - Peeling
 - Discoloration

Type II anodization

- Layer thickness 2000-10 000nm
- + Film becomes an interstitial part of the titanium
- No visible cosmetic effect

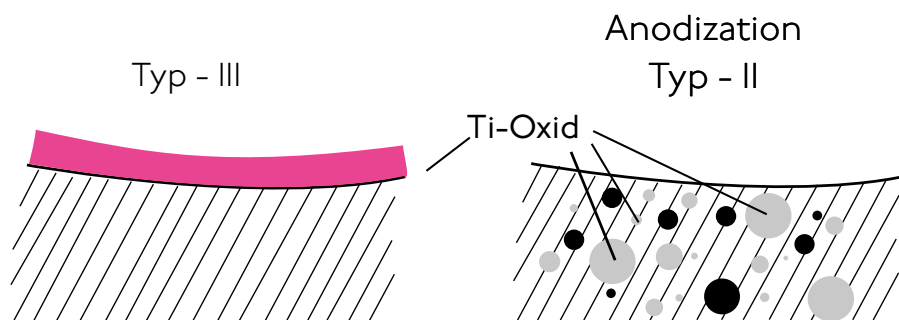


Anodization Type II leads to following benefits*

- Oxygen and silicon absorbing conversion layer
- Decrease in protein adsorption
- Closing of micro pores and micro cracks
- Reduced risk of inflammation and allergy
- Hardened titanium surface
- Reduced tendency of cold welding of titanium implants
- Increased fatigue resistance of implants
- Improved wear and friction characteristics

* White Paper: Ti6Al4V with Anodization Type II: Biological Behavior and Biomechanical Effects; Axel Baumann, Nils Zander


○ Article list

Basic Instruments

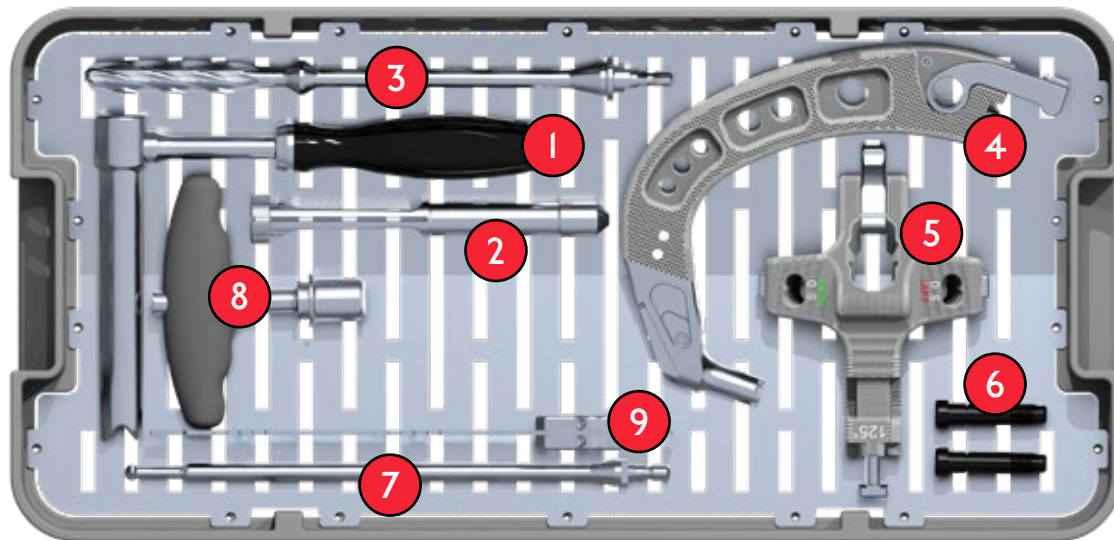


Opening & Nail Insertion

	Description	Article number
①	PF Opening Reamer Sleeve	1F0I020A
②	PF Multihole Trocar	1F0I030A
③	PF Opening Reamer	1F0I040A
④	Targeting Arm	1F0I050A
⑤	PF Targeting Module 125°	1F0I060A
⑥	PF Nail Holding Bolt	1F0I075A
⑦	PF Ball Tip Screwdriver	1F0I045A
⑧	T-Handle Zimmer Hall, Cannulated	1UI125A
⑨	PF X-Ray Ruler, Short	1F0I005A

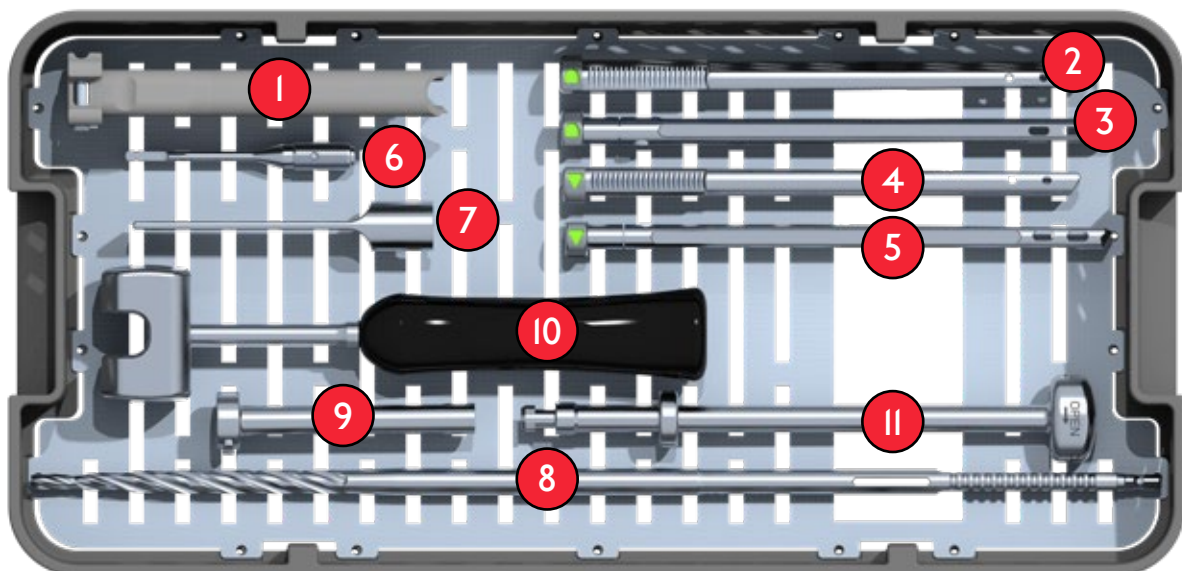

Proximal Targeting


	Description	Article number
1	PF Proximal Master Sleeve	1F0I080A
2	PF Tissue Protection Sleeve, Superior	1F0I090A
3	PF K-Wire Sleeve, Superior	1F0I100A
4	PF Tissue Protection Sleeve, Inferior	1F0I095A
5	PF K-Wire Sleeve, Inferior	1F0I105A
6	K-Wire Adapter	1F0I025A
7	PF Lag Screw Ruler	1F0I110A
8	PF Step Drill Lag Screw	1F0I115A
9	Step Drill Depth Stop	1F0I120A
10	Slotted Hammer	1UI005A
11	Impactor	1UI105A

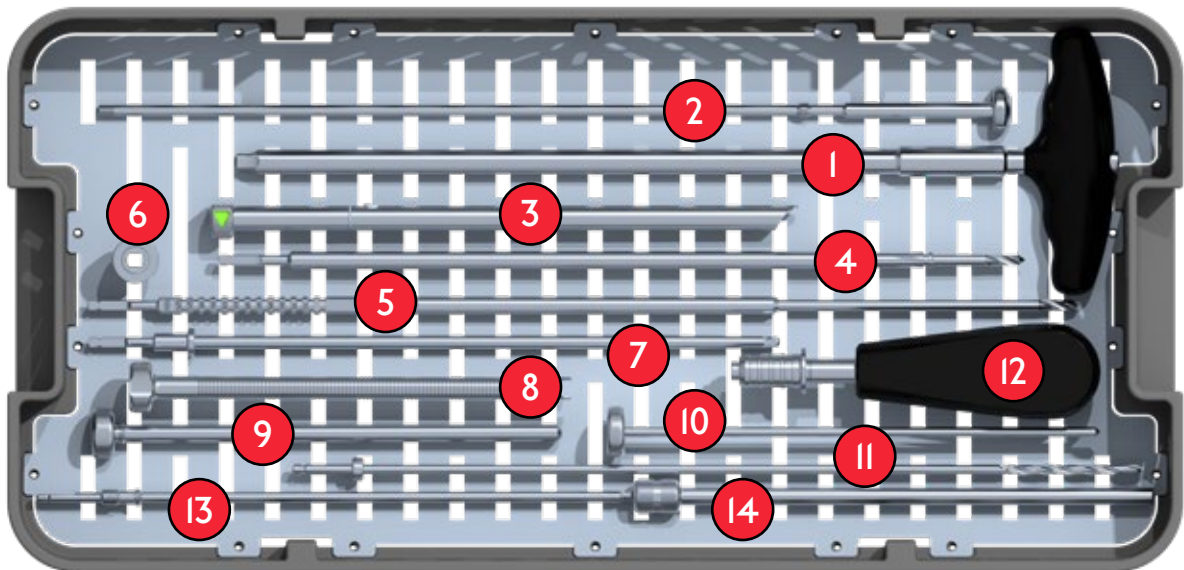

Proximal & Distal Locking


	Description	Article number
1	PF Lag Screw Driver	1F01155A
2	PF Lag Screw Driver Retaining Rod	1F01160A
3	PF Set Screw Sleeve	F01135A
4	PF Set Screw Drill	1F01140A
5	PF Set Screw Drill, optional	1F01141A
6	PF Depth Stop Set Screw Drill, optional	1F01142A
7	PF Set Screw Driver, Standard	1F01170A
8	Soft Tissue Sleeve	1U1020A
9	Drill, Sleeve, Ø4.2mm	1U1025A
10	Trocar	1U1030A
11	Drill Ø4.2mm	1U1035A-S
12	Handle, Small AO	1U1130A
13	Locking Screw Driver Shaft	1U1045A
14	Locking Screw Driver Sleeve	1U1046A

Optional Instruments

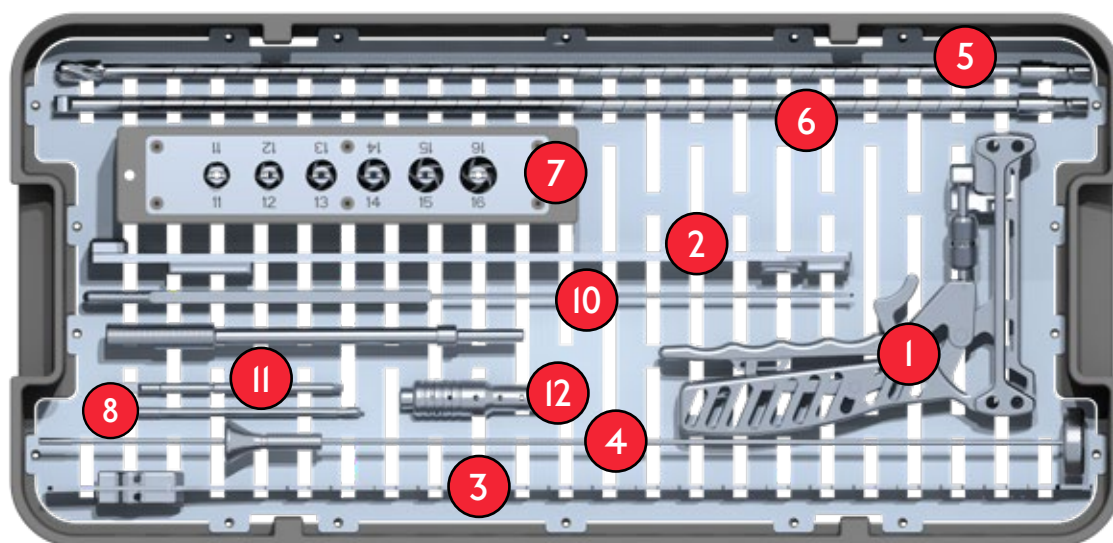


Additional Instruments for Long Nail

	Description	Article number
1	Gripper	1UI090A
2	Guide Wire Ruler	1UI010A
3	PF X-Ray Ruler, Long	1F0I010A
4	Guide Wire Pusher	1UI100A
5	Fixed Head Reamer, Ø10mm	1UI224A
6	Modular Reamer Shaft, Ø8x475mm	1UI200A
7	Modular Reamer Head, Ø11mm	1UI258A
	Modular Reamer Head, Ø12mm	1UI260A
	Modular Reamer Head, Ø13mm	1UI262A
	Modular Reamer Head, Ø14mm	1UI264A
	Modular Reamer Head, Ø15mm	1UI266A
	Modular Reamer Head, Ø16mm	1UI268A
8	Drill Freehand Ø4.2 x 120mm	1UI069A-S
9	Measuring Sleeve	1UI065A
10	Screw Gauge	1UI060A
11	Locking Screw Driver, Short	1UI050A
12	Capture Sleeve	1UI055A

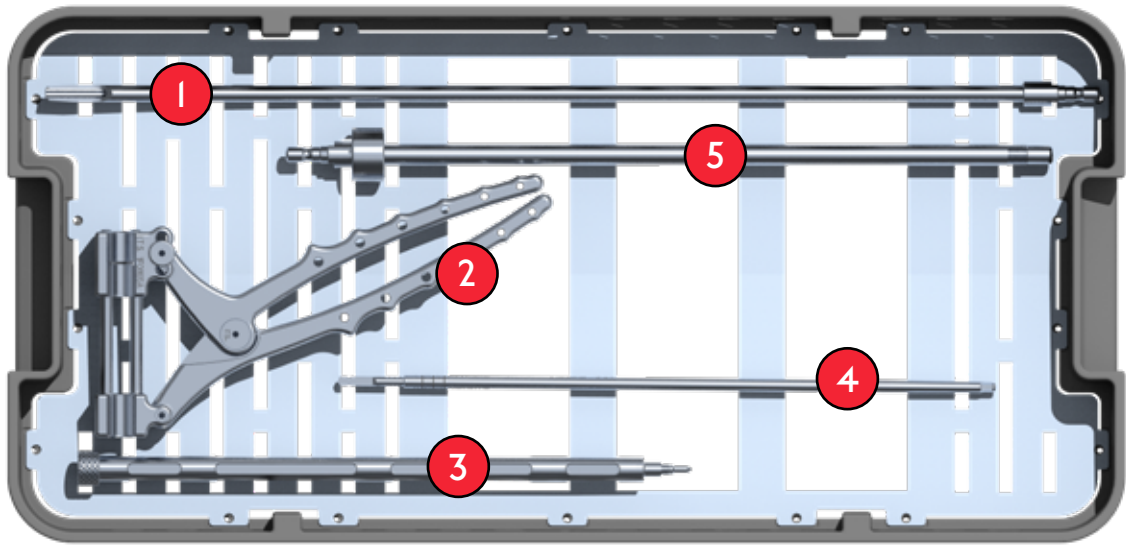

Optional Instruments I

	Description	Article number
1	Reduction Rod	1UI120A
2	PF Apositioning Instrument	1F0I165A
3	PF Compression Rod	1F0I180A
4	PF Set Screw Driver, Optional	1F0I175A
5	Extraction Rod	1UI110A

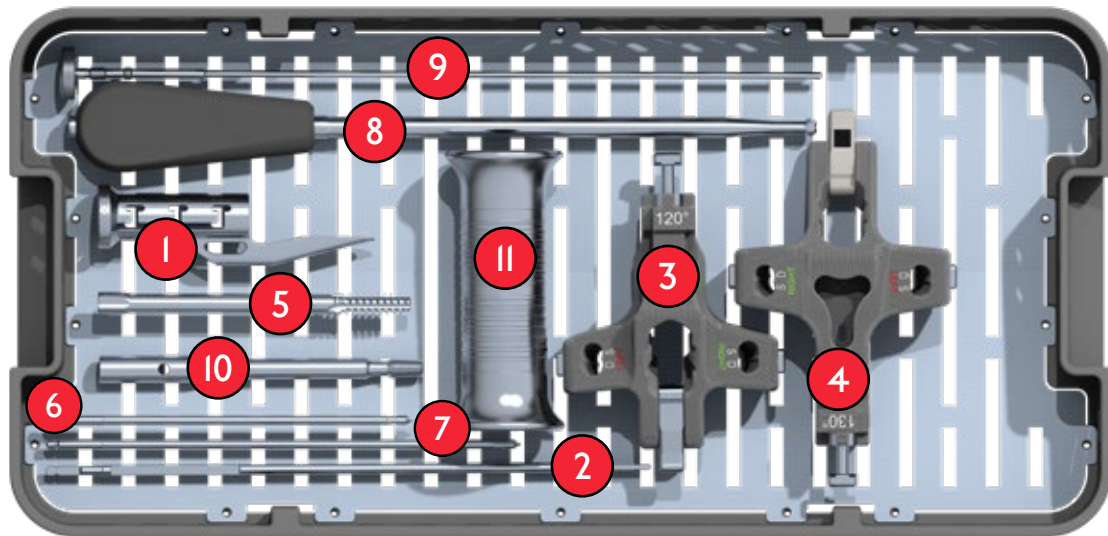

Optional Instruments 2

	Description	Article number
①	PF Opening Reamer Sleeve Rescue	1F0I035A
②	Scalpel Handle	1UI015A
③	PF Targeting Module 120°	1F0I055A
④	PF Targeting Module 130°	1F0I065A
⑤	PF Lag Screw Tap	1F0I130A
⑥	Freehand Drills 170mm	1UI070A-S
⑦	Freehand Drills 220mm	1UI071A-S
⑧	PF Ball Tip Screwdriver Self Retaining	1F0I185A
⑨	PF Retaining Rod Ball Tip Screwdriver	1F0I150A
⑩	Conical Extractor	1UI115A
⑪	Sliding Hammer	1UI135A

Nails - 120° CCD

SHORT

∅	Length (mm)	Left	Right
10mm	180	1FOL10-180-120A-S	1FOR10-180-120A-S

INTERMEDIATE

∅	Length (mm)	Left	Right
10mm	240	1FOL10-240-120A-S	1FOR10-240-120A-S

∅	Length (mm)	Left	Right
12mm	240	1FOL12-240-120A-S	1FOR12-240-120A-S



120°

LANG

∅	Length (mm)	Left	Right
9mm	260	1FOL9-260-120A-S	1FOR9-260-120A-S
	280	1FOL9-280-120A-S	1FOR9-280-120A-S
	300	1FOL9-300-120A-S	1FOR9-300-120A-S
	320	1FOL9-320-120A-S	1FOR9-320-120A-S
	340	1FOL9-340-120A-S	1FOR9-340-120A-S
	360	1FOL9-360-120A-S	1FOR9-360-120A-S
	380	1FOL9-380-120A-S	1FOR9-380-120A-S
	400	1FOL9-400-120A-S	1FOR9-400-120A-S
	420	1FOL9-420-120A-S	1FOR9-420-120A-S
	440	1FOL9-440-120A-S	1FOR9-440-120A-S
460	1FOL9-460-120A-S	1FOR9-460-120A-S	
480	1FOL9-480-120A-S	1FOR9-480-120A-S	

∅	Length (mm)	Left	Right
10mm	260	1FOL10-260-120A-S	1FOR10-260-120A-S
	280	1FOL10-280-120A-S	1FOR10-280-120A-S
	300	1FOL10-300-120A-S	1FOR10-300-120A-S
	320	1FOL10-320-120A-S	1FOR10-320-120A-S
	340	1FOL10-340-120A-S	1FOR10-340-120A-S
	360	1FOL10-360-120A-S	1FOR10-360-120A-S
	380	1FOL10-380-120A-S	1FOR10-380-120A-S
	400	1FOL10-400-120A-S	1FOR10-400-120A-S
	420	1FOL10-420-120A-S	1FOR10-420-120A-S
	440	1FOL10-440-120A-S	1FOR10-440-120A-S
460	1FOL10-460-120A-S	1FOR10-460-120A-S	
480	1FOL10-480-120A-S	1FOR10-480-120A-S	

∅	Length (mm)	Left	Right
12mm	260	1FOL12-260-120A-S	1FOR12-260-120A-S
	280	1FOL12-280-120A-S	1FOR12-280-120A-S
	300	1FOL12-300-120A-S	1FOR12-300-120A-S
	320	1FOL12-320-120A-S	1FOR12-320-120A-S
	340	1FOL12-340-120A-S	1FOR12-340-120A-S
	360	1FOL12-360-120A-S	1FOR12-360-120A-S
	380	1FOL12-380-120A-S	1FOR12-380-120A-S
	400	1FOL12-400-120A-S	1FOR12-400-120A-S
	420	1FOL12-420-120A-S	1FOR12-420-120A-S
	440	1FOL12-440-120A-S	1FOR12-440-120A-S
460	1FOL12-460-120A-S	1FOR12-460-120A-S	
480	1FOL12-480-120A-S	1FOR12-480-120A-S	

∅	Length (mm)	Left	Right
14mm	260	1FOL14-260-120A-S	1FOR14-260-120A-S
	280	1FOL14-280-120A-S	1FOR14-280-120A-S
	300	1FOL14-300-120A-S	1FOR14-300-120A-S
	320	1FOL14-320-120A-S	1FOR14-320-120A-S
	340	1FOL14-340-120A-S	1FOR14-340-120A-S
	360	1FOL14-360-120A-S	1FOR14-360-120A-S
	380	1FOL14-380-120A-S	1FOR14-380-120A-S
	400	1FOL14-400-120A-S	1FOR14-400-120A-S
	420	1FOL14-420-120A-S	1FOR14-420-120A-S
	440	1FOL14-440-120A-S	1FOR14-440-120A-S
460	1FOL14-460-120A-S	1FOR14-460-120A-S	
480	1FOL14-480-120A-S	1FOR14-480-120A-S	

Nails - 125° CCD

Short	∅	Length (mm)	LEFT	Right
	10mm	180	1FOL10-180-125A-S	1FOR10-180-125A-S

INTERMEDIATE	∅	Length (mm)	Left	Right
	10mm	240	1FOL10-240-125A-S	1FOR10-240-125A-S

INTERMEDIATE	∅	Length (mm)	Left	Right
	12mm	240	1FOL12-240-125A-S	1FOR12-240-125A-S



125°

LANG	∅	Length (mm)	Left	Right
	9mm	260	1FOL9-260-125A-S	1FOR9-260-125A-S
		280	1FOL9-280-125A-S	1FOR9-280-125A-S
		300	1FOL9-300-125A-S	1FOR9-300-125A-S
		320	1FOL9-320-125A-S	1FOR9-320-125A-S
		340	1FOL9-340-125A-S	1FOR9-340-125A-S
		360	1FOL9-360-125A-S	1FOR9-360-125A-S
		380	1FOL9-380-125A-S	1FOR9-380-125A-S
		400	1FOL9-400-125A-S	1FOR9-400-125A-S
		420	1FOL9-420-125A-S	1FOR9-420-125A-S
		440	1FOL9-440-125A-S	1FOR9-440-125A-S
		460	1FOL9-460-125A-S	1FOR9-460-125A-S
480		1FOL9-480-125A-S	1FOR9-480-125A-S	

∅	Length (mm)	Left	Right
12mm	260	1FOL12-260-125A-S	1FOR12-260-125A-S
	280	1FOL12-280-125A-S	1FOR12-280-125A-S
	300	1FOL12-300-125A-S	1FOR12-300-125A-S
	320	1FOL12-320-125A-S	1FOR12-320-125A-S
	340	1FOL12-340-125A-S	1FOR12-340-125A-S
	360	1FOL12-360-125A-S	1FOR12-360-125A-S
	380	1FOL12-380-125A-S	1FOR12-380-125A-S
	400	1FOL12-400-125A-S	1FOR12-400-125A-S
	420	1FOL12-420-125A-S	1FOR12-420-125A-S
	440	1FOL12-440-125A-S	1FOR12-440-125A-S
	460	1FOL12-460-125A-S	1FOR12-460-125A-S
	480	1FOL12-480-125A-S	1FOR12-480-125A-S

LANG	∅	Length (mm)	Left	Right
	10mm	260	1FOL10-260-125A-S	1FOR10-260-125A-S
		280	1FOL10-280-125A-S	1FOR10-280-125A-S
		300	1FOL10-300-125A-S	1FOR10-300-125A-S
		320	1FOL10-320-125A-S	1FOR10-320-125A-S
		340	1FOL10-340-125A-S	1FOR10-340-125A-S
		360	1FOL10-360-125A-S	1FOR10-360-125A-S
		380	1FOL10-380-125A-S	1FOR10-380-125A-S
		400	1FOL10-400-125A-S	1FOR10-400-125A-S
		420	1FOL10-420-125A-S	1FOR10-420-125A-S
		440	1FOL10-440-120A-S	1FOR10-440-125A-S
		460	1FOL10-460-125A-S	1FOR10-460-125A-S
480		1FOL10-480-125A-S	1FOR10-480-125A-S	

∅	Length (mm)	Left	Right
14mm	260	1FOL14-260-125A-S	1FOR14-260-125A-S
	280	1FOL14-280-125A-S	1FOR14-280-125A-S
	300	1FOL14-300-125A-S	1FOR14-300-125A-S
	320	1FOL14-320-125A-S	1FOR14-320-125A-S
	340	1FOL14-340-125A-S	1FOR14-340-125A-S
	360	1FOL14-360-125A-S	1FOR14-360-125A-S
	380	1FOL14-380-125A-S	1FOR14-380-125A-S
	400	1FOL14-400-125A-S	1FOR14-400-125A-S
	420	1FOL14-420-125A-S	1FOR14-420-125A-S
	440	1FOL14-440-125A-S	1FOR14-440-125A-S
	460	1FOL14-460-125A-S	1FOR14-460-125A-S
	480	1FOL14-480-125A-S	1FOR14-480-125A-S

Nails - 130° CCD

∅	Length (mm)	LEFT	Right
10mm	180	1FOL10-180-130A-S	1FOR10-180-130A-S

∅	Length (mm)	Left	Right
10mm	240	1FOL10-240-130A-S	1FOR10-240-130A-S

∅	Length (mm)	Left	Right
12mm	240	1FOL12-240-130A-S	1FOR12-240-130A-S



130°

∅	Length (mm)	Left	Right
9mm	260	1FOL9-260-130A-S	1FOR9-260-130A-S
	280	1FOL9-280-130A-S	1FOR9-280-130A-S
	300	1FOL9-300-130A-S	1FOR9-300-130A-S
	320	1FOL9-320-130A-S	1FOR9-320-130A-S
	340	1FOL9-340-130A-S	1FOR9-340-130A-S
	360	1FOL9-360-130A-S	1FOR9-360-130A-S
	380	1FOL9-380-130A-S	1FOR9-380-130A-S
	400	1FOL9-400-130A-S	1FOR9-400-130A-S
	420	1FOL9-420-130A-S	1FOR9-420-130A-S
	440	1FOL9-440-130A-S	1FOR9-440-130A-S
	460	1FOL9-460-130A-S	1FOR9-460-130A-S
480	1FOL9-480-130A-S	1FOR9-480-130A-S	

∅	Length (mm)	LEFT	Right
12mm	260	1FOL12-260-130A-S	1FOR12-260-130A-S
	280	1FOL12-280-130A-S	1FOR12-280-130A-S
	300	1FOL12-300-130A-S	1FOR12-300-130A-S
	320	1FOL12-320-130A-S	1FOR12-320-130A-S
	340	1FOL12-340-130A-S	1FOR12-340-130A-S
	360	1FOL12-360-130A-S	1FOR12-360-130A-S
	380	1FOL12-380-130A-S	1FOR12-380-130A-S
	400	1FOL12-400-130A-S	1FOR12-400-130A-S
	420	1FOL12-420-130A-S	1FOR12-420-130A-S
	440	1FOL12-440-130A-S	1FOR12-440-130A-S
	460	1FOL12-460-130A-S	1FOR12-460-130A-S
480	1FOL12-480-130A-S	1FOR12-480-130A-S	

∅	Length (mm)	Left	Right
10mm	260	1FOL10-260-130A-S	1FOR10-260-130A-S
	280	1FOL10-280-130A-S	1FOR10-280-130A-S
	300	1FOL10-300-130A-S	1FOR10-300-130A-S
	320	1FOL10-320-130A-S	1FOR10-320-130A-S
	340	1FOL10-340-130A-S	1FOR10-340-130A-S
	360	1FOL10-360-130A-S	1FOR10-360-130A-S
	380	1FOL10-380-130A-S	1FOR10-380-130A-S
	400	1FOL10-400-130A-S	1FOR10-400-130A-S
	420	1FOL10-420-130A-S	1FOR10-420-130A-S
	440	1FOL10-440-130A-S	1FOR10-440-130A-S
	460	1FOL10-460-130A-S	1FOR10-460-130A-S
480	1FOL10-480-130A-S	1FOR10-480-130A-S	

∅	Length (mm)	LEFT	Right
14mm	260	1FOL14-260-130A-S	1FOR14-260-130A-S
	280	1FOL14-280-130A-S	1FOR14-280-130A-S
	300	1FOL14-300-130A-S	1FOR14-300-130A-S
	320	1FOL14-320-130A-S	1FOR14-320-130A-S
	340	1FOL14-340-130A-S	1FOR14-340-130A-S
	360	1FOL14-360-130A-S	1FOR14-360-130A-S
	380	1FOL14-380-130A-S	1FOR14-380-130A-S
	400	1FOL14-400-130A-S	1FOR14-400-130A-S
	420	1FOL14-420-130A-S	1FOR14-420-130A-S
	440	1FOL14-440-130A-S	1FOR14-440-130A-S
	460	1FOL14-460-130A-S	1FOR14-460-130A-S
480	1FOL14-480-130A-S	1FOR14-480-130A-S	

DyCon® Screw Pair

Lag Screw

DyCon® Set Screw



Lag Screw

Length	Article Number
70	1F0-10-70A-S
75	1F0-10-75A-S
80	1F0-10-80A-S
85	1F0-10-85A-S
90	1F0-10-90A-S
95	1F0-10-95A-S
100	1F0-10-100A-S
105	1F0-10-105A-S
110	1F0-10-110A-S
115	1F0-10-115A-S
120	1F0-10-120A-S
125	1F0-10-125A-S
130	1F0-10-130A-S

DyCon® Set Screw

Length	Article Number
70	1F0-7-70A-S
75	1F0-7-75A-S
80	1F0-7-80A-S
85	1F0-7-85A-S
90	1F0-7-90A-S
95	1F0-7-95A-S
100	1F0-7-100A-S
105	1F0-7-105A-S
110	1F0-7-110A-S
115	1F0-7-115A-S
120	1F0-7-120A-S
125	1F0-7-125A-S
130	1F0-7-130A-S

OPTIONAL Short DyCon® Set Screw

Article Number
1F0-7-45A-S

5mm Locking Screw




Length	Article Number
25	1U1-5-25A-S
27.5	1U1-5-27A-S
30	1U1-5-30A-S
32.5	1U1-5-32A-S
35	1U1-5-35A-S
37.5	1U1-5-37A-S
40	1U1-5-40A-S
42.5	1U1-5-42A-S
45	1U1-5-45A-S
47.5	1U1-5-47A-S
50	1U1-5-50A-S
52.5	1U1-5-52A-S
55	1U1-5-55A-S
57.5	1U1-5-57A-S
60	1U1-5-60A-S
62.5	1U1-5-62A-S
65	1U1-5-65A-S
67.5	1U1-5-67A-S
70	1U1-5-70A-S
75	1U1-5-75A-S
80	1U1-5-80A-S
85	1U1-5-85A-S
90	1U1-5-90A-S
95	1U1-5-95A-S
100	1U1-5-100A-S
105	1U1-5-105A-S
110	1U1-5-110A-S
115	1U1-5-115A-S
120	1U1-5-120A-S

Accessories



Drill-Wires

	Description	Article Number
	Precision Drill-Wire, Ø3.2x390mm (3-Pack)	1F0I016A-S
	Precision Drill-Wire, Ø3.2x390mm (2-Pack)	1F0I017A-S


Ball Tip Guide Wire

	Description	Article Number
	Ball Tip Guide Wire, Ø3x800mm	1UI095A-S

Single Use Drills

	Description	Article Number
	Drill, Ø4.2mm	1UI035A-S
	Drill Freehand Locking, Ø4.2x120mm	1UI069A-S
	Drill Freehand Locking, Ø4.2x170mm	1UI070A-S
	Drill Freehand Locking, Ø4.2x220mm	1UI071A-S

OPTIONAL Endcaps

	Description	Article Number
	PF Endcap 0mm	1F0-10-30A-S
	PF Extension Endcap +5mm	1F0-15-05A-S
	PF Extension Endcap +10mm	1F0-15-10A-S
	PF Extension Endcap +15mm	1F0-15-15A-S
	PF Extension Endcap +20mm	1F0-15-20A-S

Disclaimer:

The intended users are limited to medical personnel with appropriate product training by the medical product consultants or knowledge of the surgical procedure to be applied. The medical staff must ensure that the use of I.T.S. GmbH medical devices is appropriate, taking into account the medical condition and medical history of the patient. Prior to product use, medical personnel must refer to complete information on product label and in IFU, including, but not limited to, indications, contraindications, warnings and preventative measures, and cleaning and sterilization instructions. Product availability is dependent on country registrations and clearances. For more information, please visit www.its-implant.com or contact us at office@its-implant.com. Unless otherwise noted, all information herein is the intellectual property of I.T.S. GmbH.



ITS.GmbH
Autal 28, 8301 Lassnitzhöhe, Austria
Tel.: +43 (0) 316/ 211 21 0
office@its-implant.com
www.its-implant.com



Best. Nr. INSPF- OP-0624-EN
Edition: June/2024